



Paper & Paperboard Testing Program

Summary Report #2911 S - November 2017

[Introduction to the Paper & Paperboard Interlaboratory Program](#)

[Explanation of Tables and Definitions of Terms](#)

<u>Analysis</u>	<u>Analysis Name</u>
305	Bursting Strength - Printing Papers
310	Bursting Strength - Packaging Papers
311	Tearing Strength - Newsprint
312	Tearing Strength - Printing Papers
314	Tearing Strength - Packaging Papers
320	Tensile Breaking Strength - Newsprint
321	Tensile Energy Absorption - Newsprint
322	Elongation to Break - Newsprint
325	Tensile Breaking Strength - Printing Papers
327	Tensile Energy Absorption - Printing Papers
328	Elongation to Break - Printing Papers
330	Tensile Breaking Strength - Packaging Papers
331	Tensile Energy Absorption - Packaging Papers
332	Elongation to Break - Packaging Papers
334	Folding Endurance (MIT) - Double Folds
336	Bending Resistance, Gurley Type
338	Bending Resistance, Taber Type - 0 to 10 Units
339	Bending Resistance, Taber Type - 10 to 100 Taber Units
340	Bending Resistance, Taber Type - 50 to 500 Taber Units - Recycled Paperboard
343	Z-Direction Tensile
345	Z-Direction Tensile, Recycled Paperboard
348	Internal Bond Strength - Modified Scott Mechanics
349	Internal Bond Strength - Scott Bond Models

The CTS Paper & Paperboard Interlaboratory Program

In 1969, the National Bureau of Standards (now designated the National Institute for Standards and Technology) and the Technical Association of the Pulp and Paper Industry (TAPPI) developed an interlaboratory program for paper and paperboard testing. Since 1971, Collaborative Testing Services has operated the Collaborative Reference Program for Paper and Paperboard. With hundreds of organizations from around the world participating in these tests, this program has become one of the largest of its kind. The program allows laboratories to compare the performance of their testing with that of other participating laboratories, and provides a realistic picture of the state of paper testing.

About CTS

Founded in 1971, Collaborative Testing Services, Inc. (CTS) is a privately - owned company that specializes in interlaboratory tests for a variety of industrial sectors: rubber, plastics, fasteners and metals, CKPG, paper, color and wine, as well as proficiency tests for forensic laboratories. All of the tests are designed to assist organizations in achieving and maintaining quality assurance objectives. Labs from the U.S., as well as more than 80 countries, currently participate in CTS programs.

If there are any questions on the report or testing program, please contact:

Collaborative Testing Services, Inc.
21331 Gentry Drive
Sterling, Virginia 20166 USA
+1-571-434-1925
FAX #: +1-571-434-1937
paper@cts-interlab.com

Office Hours: 8:00 a.m. - 4:30 p.m. ET

Key for Web Summary Reports (Page 1 of 2)

WebCode	Assigned laboratory identification number (temporary) used to ensure lab confidentiality while permitting a lab to locate its data in the Paper Report published on the CTS Website. The WebCode for each analysis can be found on the datasheets and in the Performance Analysis Report mailed to each participant.
Lab Mean	The average of the values obtained for each sample by the participant.
Grand Mean	The average of the LAB MEANS for all included participants. Laboratories flagged with an X or an M (see DATA FLAG column) are excluded from the GRAND MEAN.
Difference from Grand Mean	The difference of the LAB MEAN from the GRAND MEAN.
Between-Lab Standard Deviation	An indication of the precision of measurement between the laboratories. The greater the spread of the LAB MEANS about the GRAND MEAN, the larger the BETWEEN-LAB STANDARD DEVIATION (and vice versa).
Comparative Performance Value	An indication of how well a laboratory's results agree with the other participants. The CPV is a ratio indicating the number of standard deviations from the GRAND MEAN. The closer a laboratory's COMPARATIVE PERFORMANCE VALUE is to zero, the more consistent its results are with the other participants' data (and vice versa). The critical value for each CPV will vary depending on the number of labs participating in a test.
Inst Code	A code indicating the manufacturer of the instrument used to perform the test (see separate INSTRUMENT CODE LIST for each test section), if instruments are tracked.
Data Flag	DATA FLAGS are assigned based on the simultaneous analysis of both samples tested. Refer to the following chart for an explanation of each symbol:

<u>DATA FLAG</u>	<u>STATISTICALLY INCLUDED/EXCLUDED</u>	<u>ACTION REQUIRED</u>
*	INCLUDED	CAUTION - review testing procedure and monitor future results. Results fall outside 95% ellipse but within a 99% ellipse that is calculated but not drawn.
X	EXCLUDED	STOP - immediate review of data and/or testing procedure is required. Results fall outside the 99% ellipse. See specific notes following each table for more information on why the data is excluded.
M	EXCLUDED	PROCEED - lab was unable to report data for at least one sample.

Graph - For each laboratory, the LAB MEAN for the first sample (x-axis) is plotted against the LAB MEAN for the second sample (y-axis) with each point representing a laboratory. The horizontal and vertical cross-hairs are the GRAND MEANS for each sample. When 20 or more laboratories are in the statistics, an ellipse is also drawn so that 95% of the time a randomly selected laboratory will be included inside the ellipse. Plotted data flags are explained on the previous page.

Common Problems Highlighted in Footnotes

1. **Extreme data** - The laboratory's results for one or both samples are so inconsistent with those of the other participants that the lab mean(s) fall outside the plot. The participant is advised to immediately review his data and/or testing procedure.
2. **Systematic bias** - The laboratory's results are either consistently high or low for both samples when compared to the other participants (the plotted point falls near the top or bottom of the ellipse). This indicates that the participant is performing the test with a constant bias. Causes of systematic errors include improper calibration, the particular make/model of equipment or a modification to the testing procedure.
3. **Inconsistency in testing between samples/sample sets** - The laboratory's results indicate that there are differences in the way the two samples tested (the plotted point falls to the side of the ellipse). This type of error may be attributed to the analyst deviating from the procedure when testing one of the samples or a material interaction occurrence with the instrument or room conditions. The inconsistency is reflected in the CPVs for the two samples, such as a +1.5 CPV for sample A and a -2.2 CPV for sample B. CTS also will specify if the laboratory's data for one sample are high/low compared to the other participants. If this inconsistency is slight, the lab's plotted point will be an * that falls on the edge of the ellipse.
4. **Inconsistency in testing within a sample** - The laboratory's within-lab standard deviation for a specified sample is high when compared to the other participants, often causing the lab's plotted point to fall outside of the ellipse.

Labs flagged with an * are not typically included in the footnotes of a data table. These labs may locate their position in the control ellipse and use the definitions above to help identify the type of testing error. An * should serve as a caution flag, a "yellow light", to a lab. If this error is repeated in future rounds, a lab may need to stop and review its testing procedures. The initial data flag is not cause for alarm. Interlaboratory tests conducted at regular intervals permit a lab to recognize trends in testing.



Paper & Paperboard Interlaboratory Testing Program
Analysis 305
Bursting Strength - Printing Papers
TAPPI Official Test Method T403

Report #2911S,
November 2017

WebCode	Data Flag	Sample SA49			Sample SA50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
2G7Y4H		19.83	-2.03	-1.01	21.32	-1.19	-0.64
2K76KA		21.44	-0.43	-0.21	21.61	-0.90	-0.49
778RCF		20.13	-1.74	-0.86	21.77	-0.75	-0.40
7XXAUG		18.00	-3.86	-1.91	19.10	-3.42	-1.84
7YQGZY		23.69	1.83	0.91	23.56	1.05	0.57
92UQ72	X	16.94	-4.92	-2.44	16.90	-5.62	-3.03
CT3K2Q		20.96	-0.90	-0.45	22.10	-0.41	-0.22
DJB9B9		23.83	1.97	0.98	24.89	2.38	1.28
FM7YJE		20.97	-0.89	-0.44	20.83	-1.69	-0.91
JRMTN2		23.84	1.98	0.98	23.79	1.27	0.69
JVACU6		24.05	2.19	1.08	24.63	2.11	1.14
N3RAQE		23.69	1.83	0.90	23.37	0.86	0.46
NBLFJF		17.72	-4.14	-2.05	18.79	-3.73	-2.01
QCBP6T		23.95	2.09	1.03	24.64	2.13	1.15
RPDFLR		23.30	1.44	0.71	24.00	1.48	0.80
TQHKE7		22.19	0.33	0.16	23.79	1.27	0.69
TVUHW2	X	402.48	380.62	188.39	419.89	397.37	214.46
VD46K7		21.73	-0.14	-0.07	22.16	-0.35	-0.19
WFAULU		23.95	2.08	1.03	24.63	2.11	1.14
XLUARC		21.77	-0.09	-0.05	22.25	-0.27	-0.14
XX7LWU		20.35	-1.51	-0.75	20.55	-1.97	-1.06

Summary Statistics	Sample SA49	Sample SA50
Grand Means	21.86 psi	22.52 psi
Std Dev Btwn Labs	2.02 psi	1.85 psi
Statistics based on 19 of 21 reporting participants.		

Comments on Assigned Data Flags for Test #305

92UQ72 (X) - Data for sample SA50 are low.

TVUHW2 (X) - Extreme Data.




Paper & Paperboard Interlaboratory Testing Program
Analysis 305
Bursting Strength - Printing Papers
TAPPI Official Test Method T403

Report #2911S,
November 2017

Grand Mean Sample SA49 = 21.862
psi

Grand Mean Sample SA50 = 22.515
psi

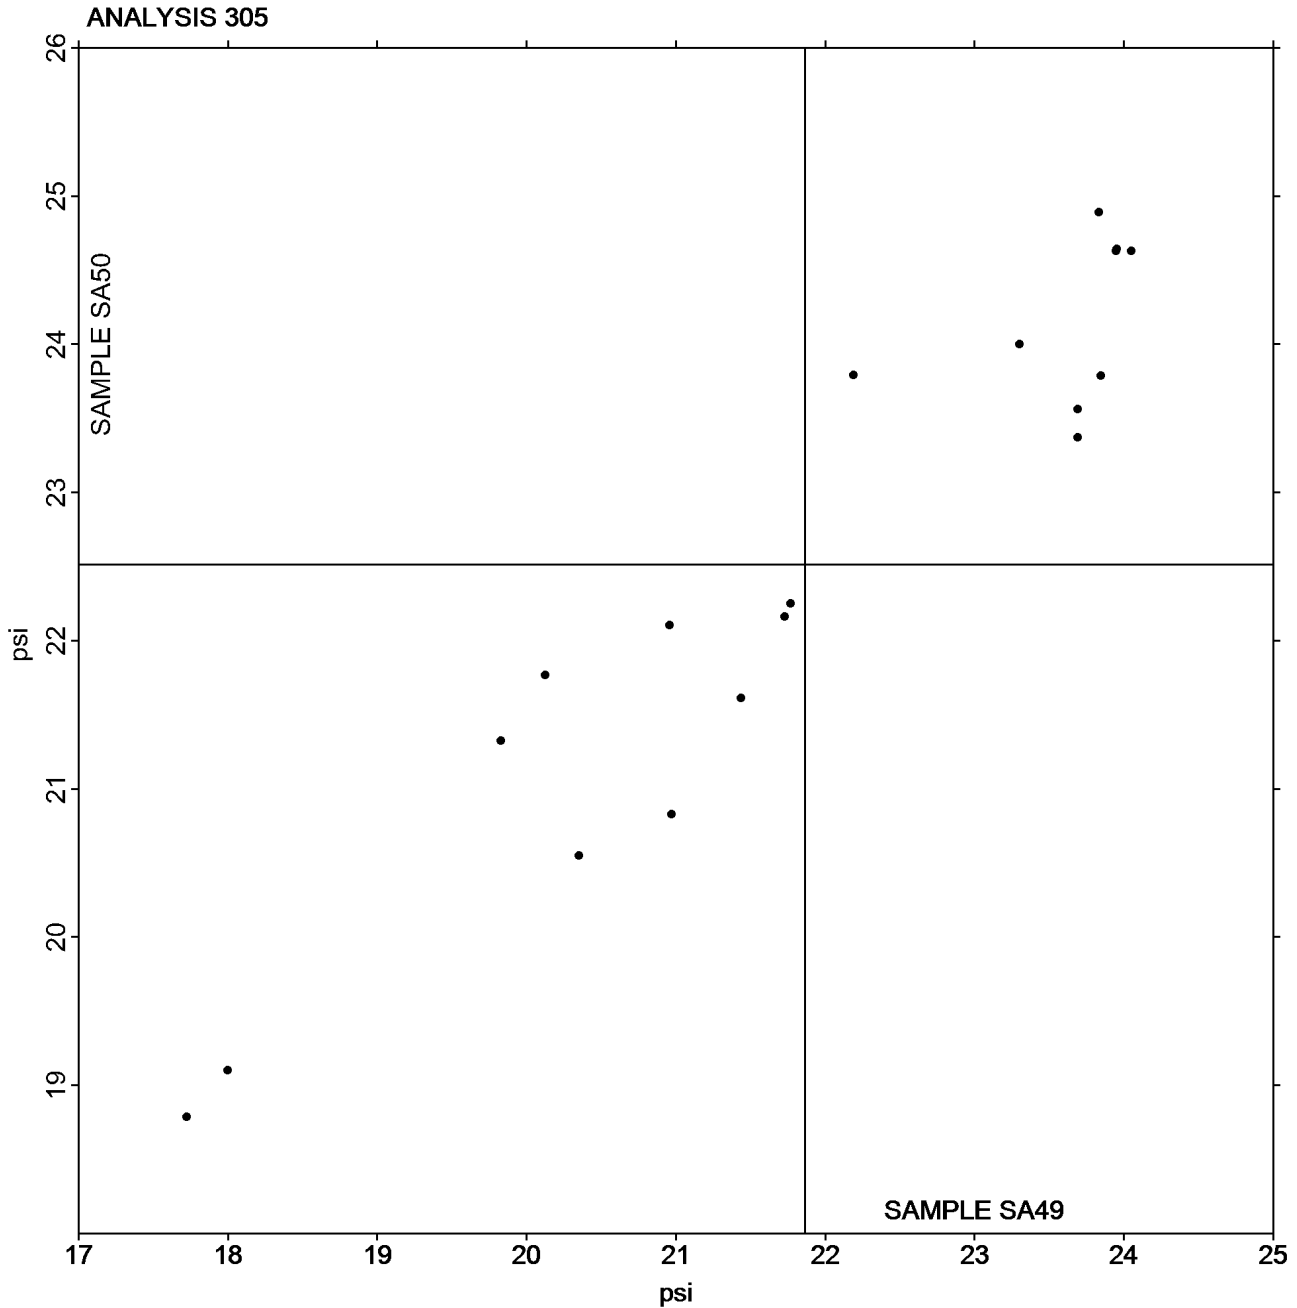

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 310
Bursting Strength - Packaging Papers
TAPPI Official Test Method T403

Report #2911S,
November 2017

WebCode	Data Flag	Sample SB49			Sample SB50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
62XC6C		88.46	-2.03	-0.35	77.89	-6.20	-1.17
6T9NAA		84.60	-5.89	-1.03	80.90	-3.18	-0.60
7YQGZY		90.75	0.26	0.04	81.18	-2.90	-0.55
8Y2PGD		87.90	-2.59	-0.45	80.90	-3.18	-0.60
99RMQJ		87.58	-2.91	-0.51	81.00	-3.08	-0.58
9FAQZ8		88.53	-1.95	-0.34	81.08	-3.01	-0.57
BJMDPW		89.85	-0.64	-0.11	82.89	-1.19	-0.23
C7BE89		96.60	6.11	1.07	88.70	4.62	0.87
DD8GXR		88.06	-2.43	-0.42	80.81	-3.28	-0.62
FBTUCH		91.04	0.55	0.10	85.25	1.17	0.22
FEU3E8		78.60	-11.89	-2.08	71.40	-12.68	-2.40
FLALWL		83.46	-7.03	-1.23	77.24	-6.85	-1.30
H8HT3V		90.23	-0.26	-0.05	85.37	1.29	0.24
JHL7YP		91.00	0.51	0.09	85.20	1.12	0.21
JRMTN2		90.66	0.18	0.03	85.53	1.44	0.27
MBQLZQ		84.51	-5.97	-1.04	79.67	-4.41	-0.84
MDXUBV	X	104.34	13.85	2.42	101.90	17.81	3.37
N3RAQE		88.38	-2.11	-0.37	86.03	1.95	0.37
NH338Q		83.70	-6.79	-1.19	77.30	-6.78	-1.28
P4DMGV		88.20	-2.29	-0.40	80.75	-3.33	-0.63
QC8Z3G	*	81.79	-8.70	-1.52	81.54	-2.54	-0.48
QJ8K6C		92.42	1.93	0.34	85.49	1.40	0.27
QTX3JK		94.31	3.82	0.67	86.78	2.70	0.51
QVKMNP		96.00	5.51	0.96	89.60	5.52	1.04
UCX8W6	*	102.05	11.56	2.02	90.16	6.08	1.15
XX7LWU		94.52	4.03	0.70	87.80	3.72	0.70
Y63WN4		95.12	4.64	0.81	91.97	7.89	1.49
YKPJPL		96.90	6.41	1.12	91.10	7.01	1.33
Z38V2D		103.70	13.21	2.31	95.60	11.52	2.18
ZXY8NB		95.23	4.74	0.83	89.33	5.25	0.99

Summary Statistics	Sample SB49	Sample SB50
Grand Means	90.49 psi	84.08 psi
Std Dev Btwn Labs	5.73 psi	5.29 psi
Statistics based on 29 of 30 reporting participants.		

Comments on Assigned Data Flags for Test #310

MDXUBV (X) - Data for sample SB50 are high.



Paper & Paperboard Interlaboratory Testing Program
Analysis 311
Tearing Strength - Newsprint
TAPPI Official Test Method T414

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SK49</u>			<u>Sample SK50</u>		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
78HWMH		27.18	-1.99	-0.61	18.52	-1.79	-0.63
BWAKKC		34.16	4.99	1.52	24.43	4.12	1.46
DD7RR9		33.70	4.53	1.38	24.40	4.09	1.44
GYUK3E		27.44	-1.73	-0.53	18.86	-1.45	-0.51
JVACU6		26.46	-2.71	-0.83	18.50	-1.81	-0.64
LP8D86		27.51	-1.66	-0.51	18.09	-2.22	-0.78
N3RAQE		27.75	-1.42	-0.43	19.36	-0.95	-0.33

Summary Statistics	<u>Sample SK49</u>	<u>Sample SK50</u>
Grand Means	29.17 Grams	20.31 Grams
Std Dev Btwn Labs	3.28 Grams	2.83 Grams
Statistics based on 7 of 7 reporting participants.		




Paper & Paperboard Interlaboratory Testing Program
Analysis 311
Tearing Strength - Newsprint
TAPPI Official Test Method T414

Report #2911S,
November 2017

Grand Mean Sample SK49 = 29.171
Grams

Grand Mean Sample SK50 = 20.310
Grams

ANALYSIS 311

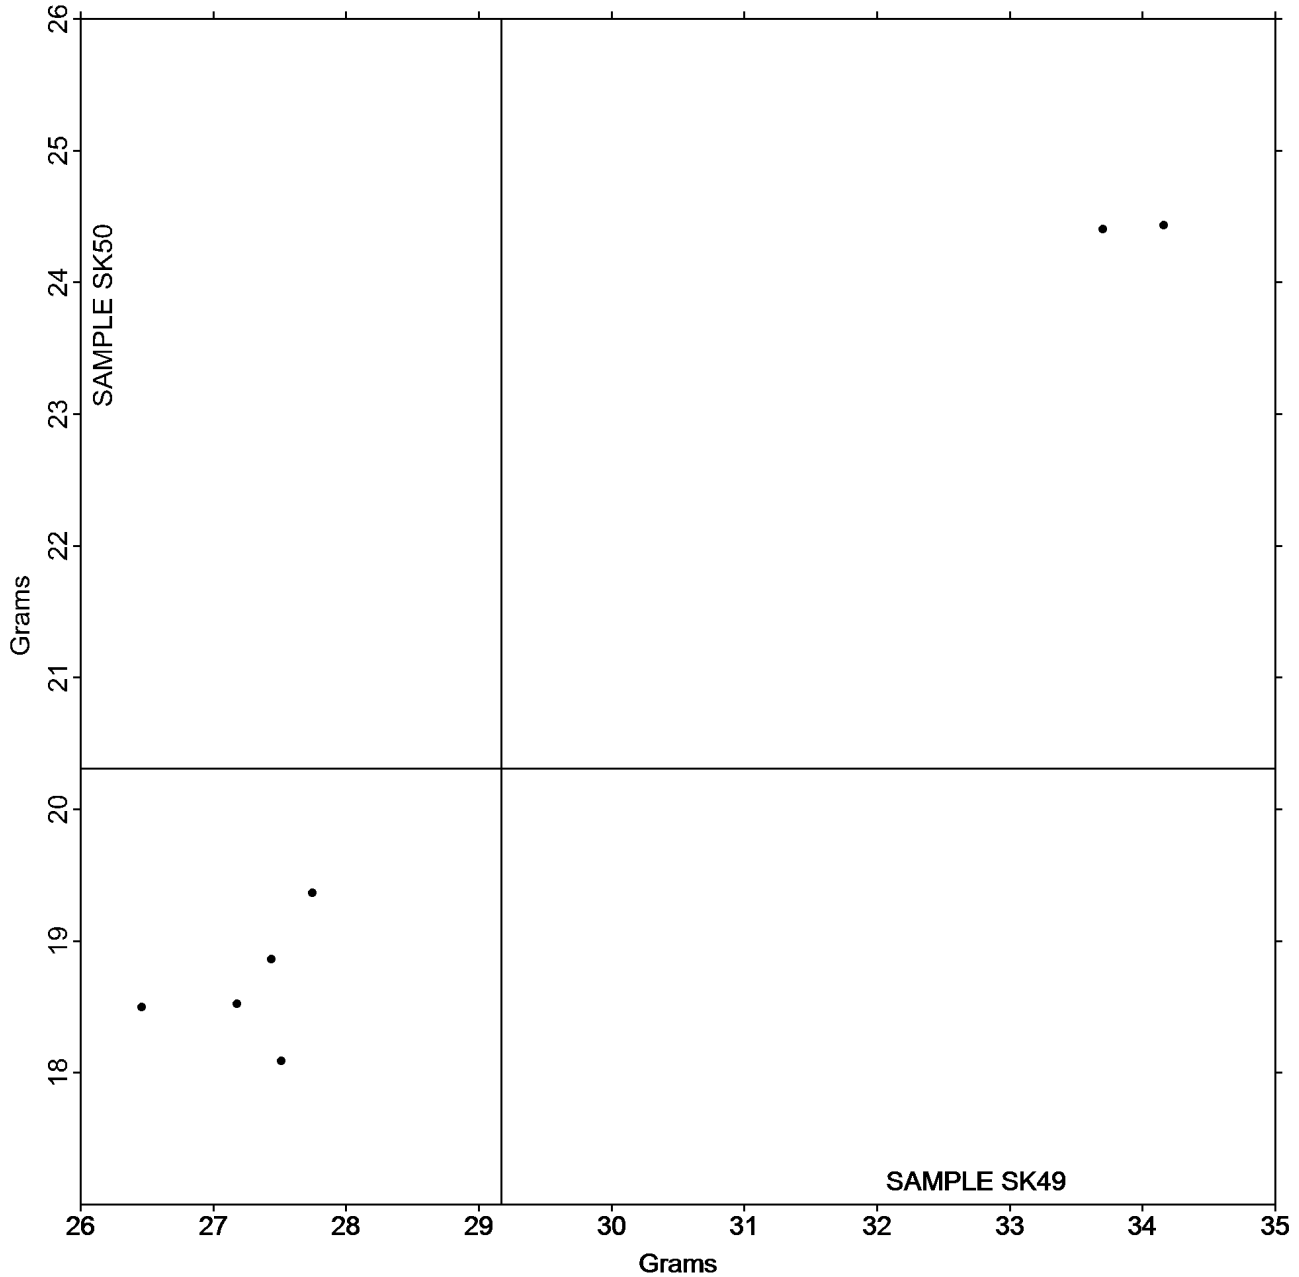

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 312
Tearing Strength - Printing Papers
TAPPI Official Test Method T414

Report #2911S,
November 2017

WebCode	Data Flag	Sample SC49			Sample SC50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
2E292A		48.26	0.24	0.08	46.58	-0.35	-0.12
2G7Y4H		45.49	-2.53	-0.87	44.03	-2.90	-0.98
2K76KA		50.36	2.34	0.81	47.60	0.66	0.22
2V4BCM	X	59.10	11.08	3.83	58.76	11.82	3.98
3GMFWQ		52.43	4.41	1.52	51.36	4.43	1.49
3X9V39		48.46	0.44	0.15	47.13	0.20	0.07
62XC6C		51.76	3.74	1.29	50.96	4.03	1.36
778RCF		51.44	3.42	1.18	50.18	3.25	1.09
7N7A2A	X	51.40	3.38	1.17	43.88	-3.05	-1.03
7XXAUG		46.96	-1.06	-0.36	46.64	-0.29	-0.10
7YQGZY		51.15	3.13	1.08	51.62	4.69	1.58
874MCW		44.28	-3.74	-1.29	42.58	-4.35	-1.47
883W7E		45.20	-2.82	-0.97	43.50	-3.43	-1.16
8Y2PGD		43.06	-4.96	-1.71	42.93	-4.00	-1.35
92UQ72		49.26	1.24	0.43	47.67	0.74	0.25
99RMQJ		51.78	3.76	1.30	51.04	4.10	1.38
9JNN79	*	51.58	3.56	1.23	48.42	1.48	0.50
BJMDPW		49.92	1.90	0.66	49.43	2.49	0.84
CT3K2Q		48.11	0.09	0.03	46.92	-0.02	-0.01
DJB NB9		47.68	-0.34	-0.12	46.16	-0.77	-0.26
EQB6LE		47.46	-0.56	-0.19	47.15	0.22	0.07
FCMM7F		52.80	4.78	1.65	50.78	3.85	1.30
FM7YJE		47.72	-0.30	-0.10	46.48	-0.45	-0.15
FRFET3		42.30	-5.72	-1.97	41.76	-5.17	-1.74
FZBE6A		49.41	1.40	0.48	46.70	-0.24	-0.08
GTNPJE		52.40	4.38	1.51	51.00	4.07	1.37
GZP2GW	X	51.44	3.42	1.18	44.14	-2.79	-0.94
H8HT3V		48.32	0.30	0.10	45.96	-0.97	-0.33
JRMTN2		44.69	-3.32	-1.15	44.27	-2.67	-0.90
N3RAQE		48.45	0.43	0.15	48.23	1.30	0.44
NBLFJF		49.38	1.36	0.47	49.40	2.47	0.83
P4DMGV		44.34	-3.68	-1.27	43.20	-3.73	-1.26
PP234X		43.58	-4.44	-1.53	42.87	-4.06	-1.37
Q76ULT		48.48	0.46	0.16	46.96	0.03	0.01
QC8Z3G		50.41	2.40	0.83	50.73	3.80	1.28
QCBP6T		44.12	-3.90	-1.35	44.19	-2.74	-0.92
QTX3JK		46.83	-1.19	-0.41	45.83	-1.10	-0.37
QVKMNP		47.60	-0.42	-0.14	45.60	-1.33	-0.45
RPDFLR		51.35	3.33	1.15	51.60	4.67	1.57
TQHKE7		48.50	0.48	0.17	47.70	0.77	0.26



Paper & Paperboard Interlaboratory Testing Program
Analysis 312
Tearing Strength - Printing Papers
TAPPI Official Test Method T414

Report #2911S,
November 2017

WebCode	Data Flag	Sample SC49			Sample SC50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
TVUHW2		49.80	1.78	0.62	48.80	1.87	0.63
U46RAL	X	69.80	21.78	7.52	63.20	16.27	5.48
UQHPP9		49.20	1.18	0.41	47.52	0.59	0.20
VD46K7		48.82	0.81	0.28	47.48	0.55	0.18
WFAULU		44.77	-3.25	-1.12	43.96	-2.97	-1.00
WFNFVV		44.10	-3.92	-1.35	43.30	-3.63	-1.22
X93RPR	*	42.46	-5.56	-1.92	39.73	-7.20	-2.43
XRYBPK		46.12	-1.90	-0.65	45.28	-1.65	-0.56
YKPJPL		50.72	2.70	0.93	50.59	3.66	1.23
ZL9F48		47.48	-0.54	-0.19	47.10	0.17	0.06

Summary Statistics	Sample SC49	Sample SC50
Grand Means	48.02 Grams	46.93 Grams
Std Dev Btwn Labs	2.90 Grams	2.97 Grams

Statistics based on 46 of 50 reporting participants.

Comments on Assigned Data Flags for Test #312

- 2V4BCM (X) - Data for both samples are high. Possible Systematic Error. Inconsistent within the determinations of both samples.
- GZP2GW (X) - Inconsistent in testing between samples. Inconsistent within the determinations of both samples.
- 7N7A2A (X) - Inconsistent in testing between samples. Inconsistent within the determinations of sample SC49.
- U46RAL (X) - Extreme Data.

Analysis Notes:

WFAULU - One determination removed from the Lab Mean of Sample SC49 per Grubb's Test at 1% risk (TAPPI 1205).




Paper & Paperboard Interlaboratory Testing Program
Analysis 312
Tearing Strength - Printing Papers
TAPPI Official Test Method T414

Report #2911S,
November 2017

Grand Mean Sample SC49 = 48.017
Grams

Grand Mean Sample SC50 = 46.933
Grams

ANALYSIS 312

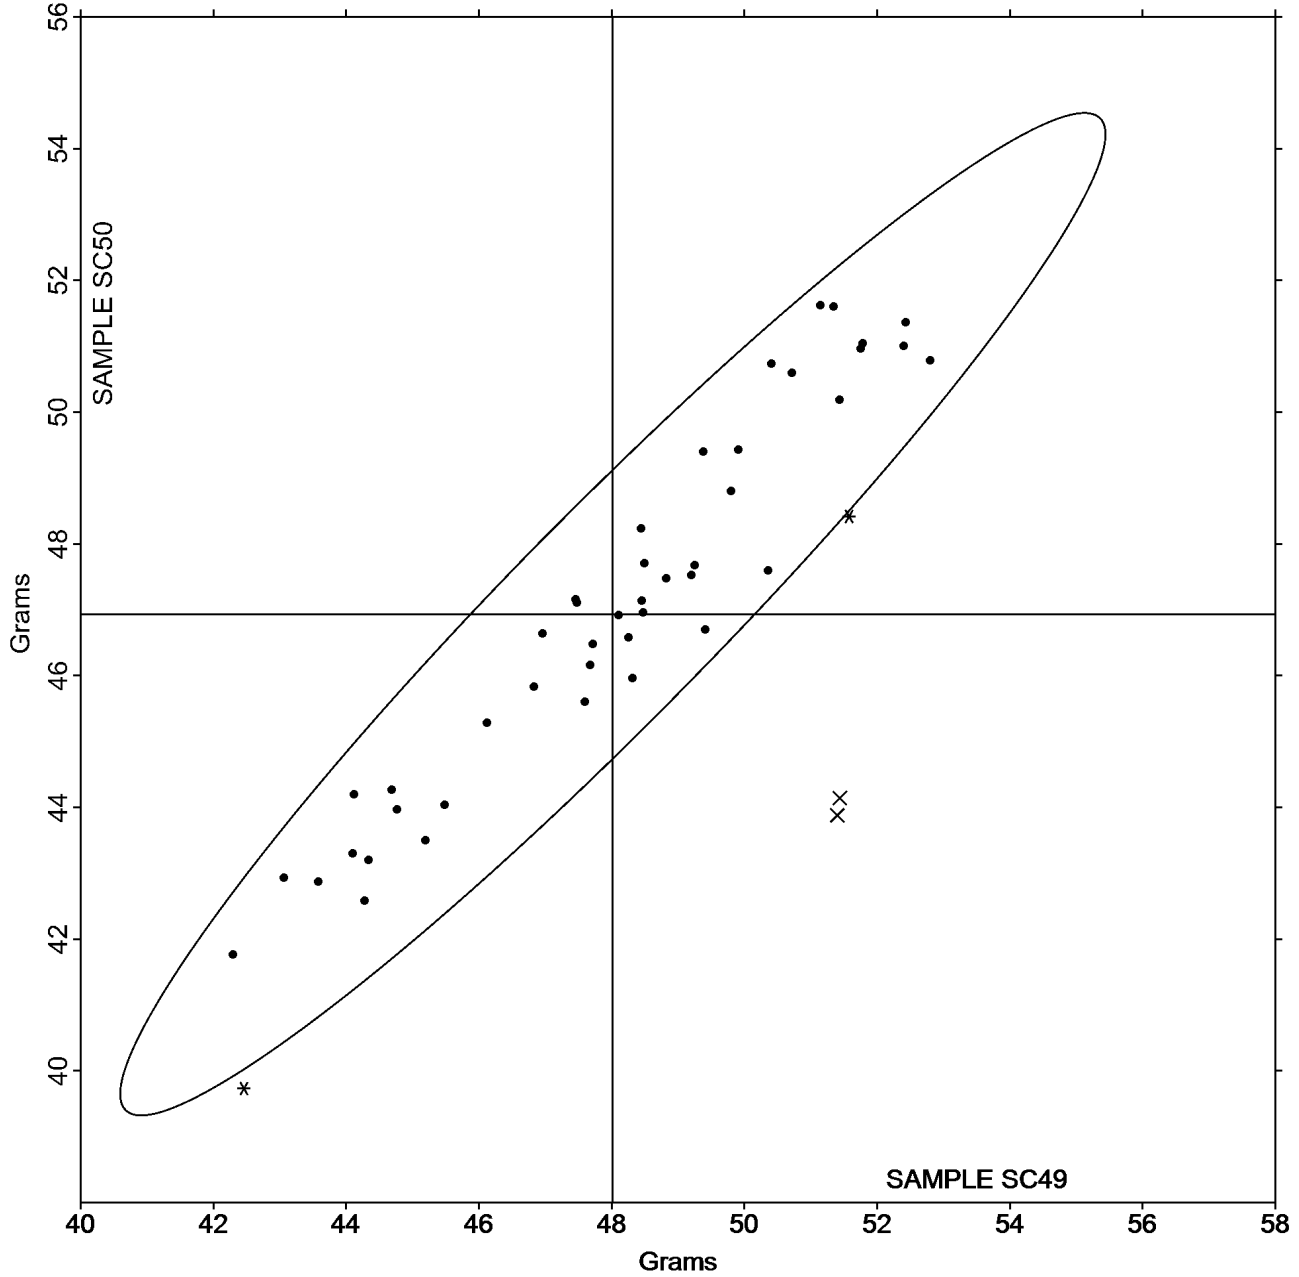



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 314

Tearing Strength - Packaging Papers

TAPPI Official Test Method T414

WebCode	Data Flag	Sample SD49			Sample SD50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
4FPJP9		177.7	6.0	0.40	174.4	1.3	0.09
4YHM79		163.2	-8.5	-0.55	170.6	-2.5	-0.18
6T9NAA		180.0	8.4	0.55	172.6	-0.5	-0.04
96M2TK		170.6	-1.0	-0.07	172.5	-0.6	-0.04
9FAQZ8		151.0	-20.6	-1.35	150.6	-22.5	-1.64
9JNN79		182.3	10.7	0.70	177.8	4.7	0.34
B7VM6R		167.5	-4.1	-0.27	168.6	-4.5	-0.32
BW9TNP		193.9	22.3	1.46	194.6	21.5	1.57
C6YQT4		139.1	-32.6	-2.13	141.6	-31.5	-2.29
C7BE89		182.4	10.8	0.71	175.2	2.1	0.15
D6TVM3		171.6	0.0	0.00	180.4	7.3	0.53
DD8GXR		183.6	12.0	0.79	180.5	7.4	0.54
EQB6LE		174.7	3.1	0.20	178.8	5.7	0.42
FBTUCH		187.6	16.0	1.05	197.0	23.9	1.74
FEU3E8	X	219.1	47.5	3.11	216.1	43.0	3.14
FLALWL		178.0	6.4	0.42	178.0	4.9	0.36
FX7P3Z	X	110.7	-60.9	-3.99	119.7	-53.4	-3.90
GAWZRJ		175.7	4.1	0.27	173.6	0.6	0.04
GL7FVH		167.9	-3.7	-0.24	172.2	-0.9	-0.06
JHL7YP		170.1	-1.5	-0.10	173.7	0.6	0.04
MDXUBV		186.0	14.3	0.94	181.5	8.4	0.62
MGUPN4		145.6	-26.0	-1.70	157.2	-15.9	-1.16
MYDGVF		156.6	-15.1	-0.99	159.4	-13.7	-1.00
N3RAQE		178.3	6.7	0.44	180.3	7.2	0.53
NH338Q	X	10.5	-161.1	-10.55	10.9	-162.2	-11.83
Q98ULQ	X	124.3	-47.3	-3.10	118.8	-54.3	-3.96
QJ8K6C	X	200.7	29.1	1.90	222.2	49.1	3.58
QUAHDL		165.7	-5.9	-0.39	162.9	-10.2	-0.74
QVKMNP	X	85.4	-86.2	-5.64	94.8	-78.3	-5.71
RDLP49		201.4	29.8	1.95	198.2	25.1	1.83
UCX8W6		176.4	4.8	0.31	172.0	-1.1	-0.08
VT3WPV		160.1	-11.5	-0.75	162.3	-10.7	-0.78
WLVTUTU		205.2	33.5	2.20	206.2	33.1	2.42
XQP2XN		170.5	-1.1	-0.07	170.9	-2.2	-0.16
XUNH9W		154.1	-17.5	-1.15	157.9	-15.2	-1.11
XX7LWU		161.2	-10.4	-0.68	170.0	-3.1	-0.23
Y46LT2		179.5	7.8	0.51	182.7	9.6	0.70
Z9TUAD		148.3	-23.3	-1.52	159.4	-13.7	-1.00
ZXY8NB		157.7	-14.0	-0.91	158.2	-14.9	-1.09



Analysis 314

Tearing Strength - Packaging Papers

TAPPI Official Test Method T414

Summary Statistics	Sample SD49	Sample SD50
Grand Means	171.62 Grams	173.09 Grams
Stnd Dev Btwn Labs	15.28 Grams	13.71 Grams
Statistics based on 33 of 39 reporting participants.		

Comments on Assigned Data Flags for Test #314

FEU3E8 (X) - Data for both samples are high. Possible Systematic Error.

Q98ULQ (X) - Data for both samples are low. Possible Systematic Error.

FX7P3Z (X) - Data for both samples are low. Possible Systematic Error. Inconsistent within the determinations of sample SD49.

QVKMNP (X) - Data for both samples are low. Possible Systematic Error.

QJ8K6C (X) - Data for sample SD50 are high. Inconsistent within the determinations of both samples.

NH338Q (X) - Extreme Data.

Analysis Notes:


9FAQZ8 - Data appear to be off by a factor of .25; data converted by CTS (x4).



Analysis 314
Tearing Strength - Packaging Papers
TAPPI Official Test Method T414

Grand Mean Sample SD49 = 171.62
Grams

Grand Mean Sample SD50 = 173.09
Grams

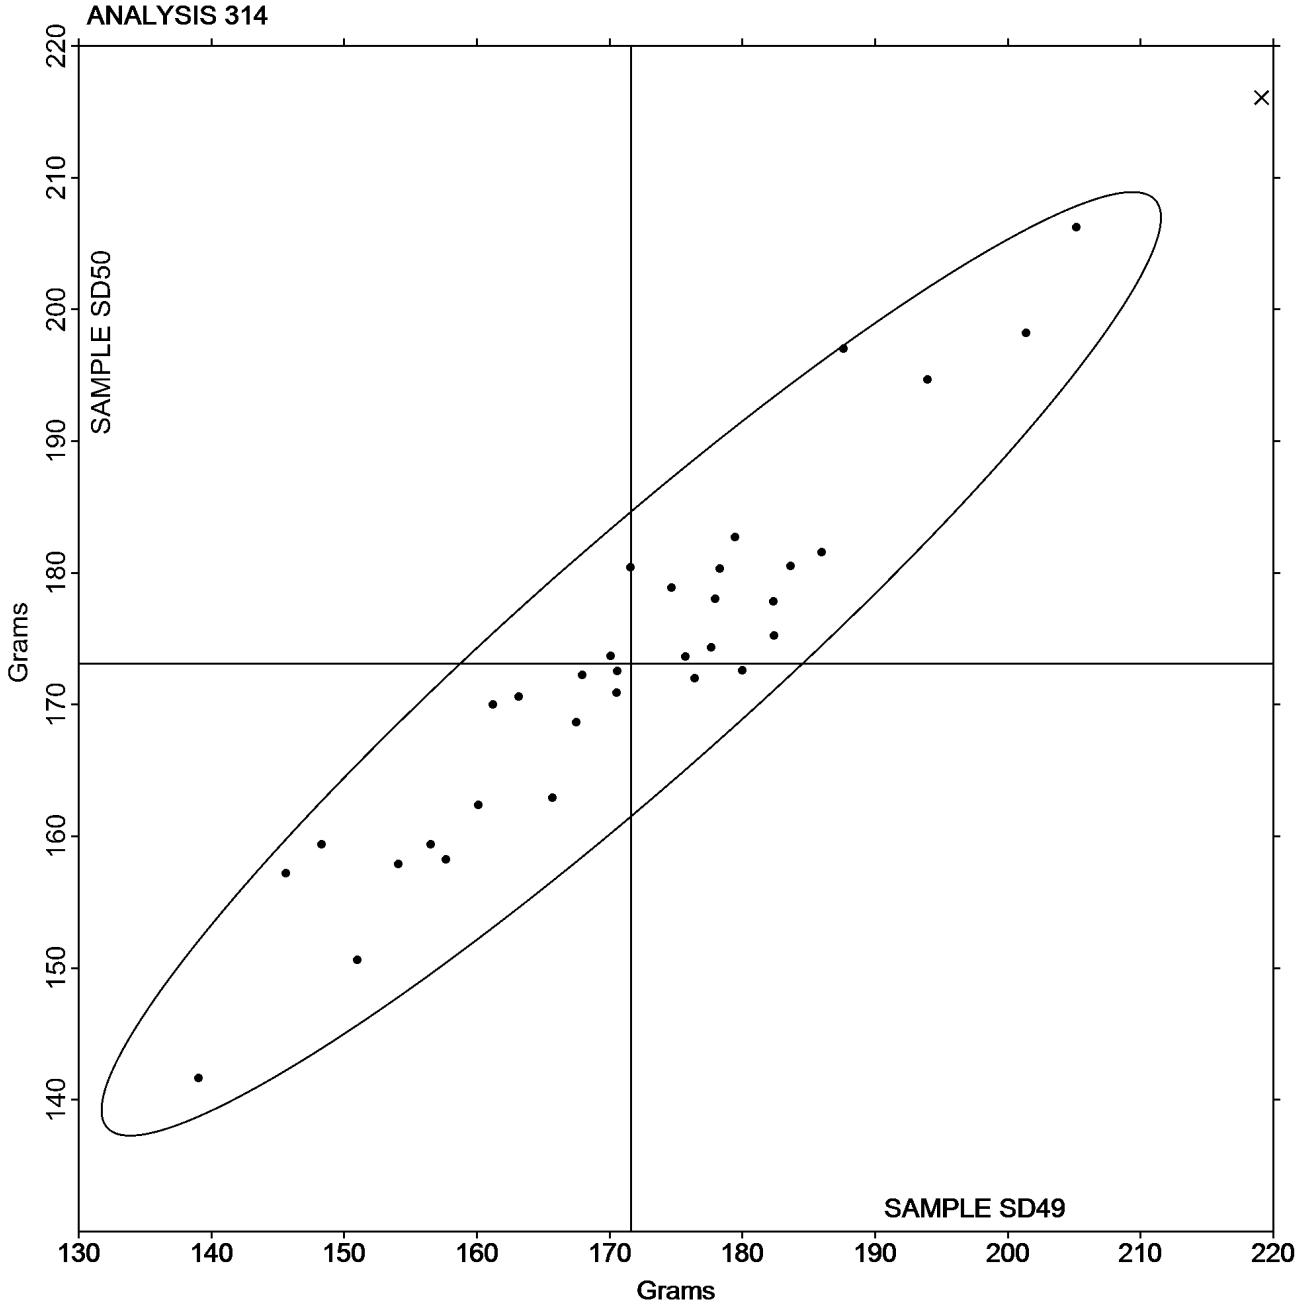



Paper & Paperboard Interlaboratory Testing Program
Analysis 320
Tensile Breaking Strength - Newsprint
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SR49</u>			<u>Sample SR50</u>		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
76YQ6M		2.793	-0.198	-0.94	2.025	-0.168	-1.01
78HWMH		3.044	0.052	0.25	1.996	-0.197	-1.18
9JNN79		2.859	-0.133	-0.63	2.213	0.020	0.12
BWAKKC		2.960	-0.032	-0.15	2.254	0.060	0.36
DD7RR9		2.951	-0.040	-0.19	2.145	-0.048	-0.29
DMBWJP		3.510	0.518	2.46	2.609	0.416	2.49
GYUK3E		2.909	-0.083	-0.39	2.194	0.001	0.00
JRMTN2		3.017	0.025	0.12	2.196	0.003	0.02
JVACU6		3.088	0.096	0.46	2.303	0.109	0.66
LP8D86		2.654	-0.338	-1.60	1.964	-0.229	-1.38
TQHKE7		3.186	0.194	0.92	2.243	0.050	0.30
XLUARC		2.832	-0.160	-0.76	2.086	-0.108	-0.65
Z38V2D		3.088	0.096	0.46	2.286	0.093	0.56

Summary Statistics	<u>Sample SR49</u>	<u>Sample SR50</u>
Grand Means	2.99 kN/m	2.19 kN/m
Std Dev Btwn Labs	0.21 kN/m	0.17 kN/m
Statistics based on 13 of 13 reporting participants.		




Analysis 320

Tensile Breaking Strength - Newsprint

TAPPI Official Test Method T494

Grand Mean Sample SR49 = 2.9916
kN/m

Grand Mean Sample SR50 = 2.1934
kN/m

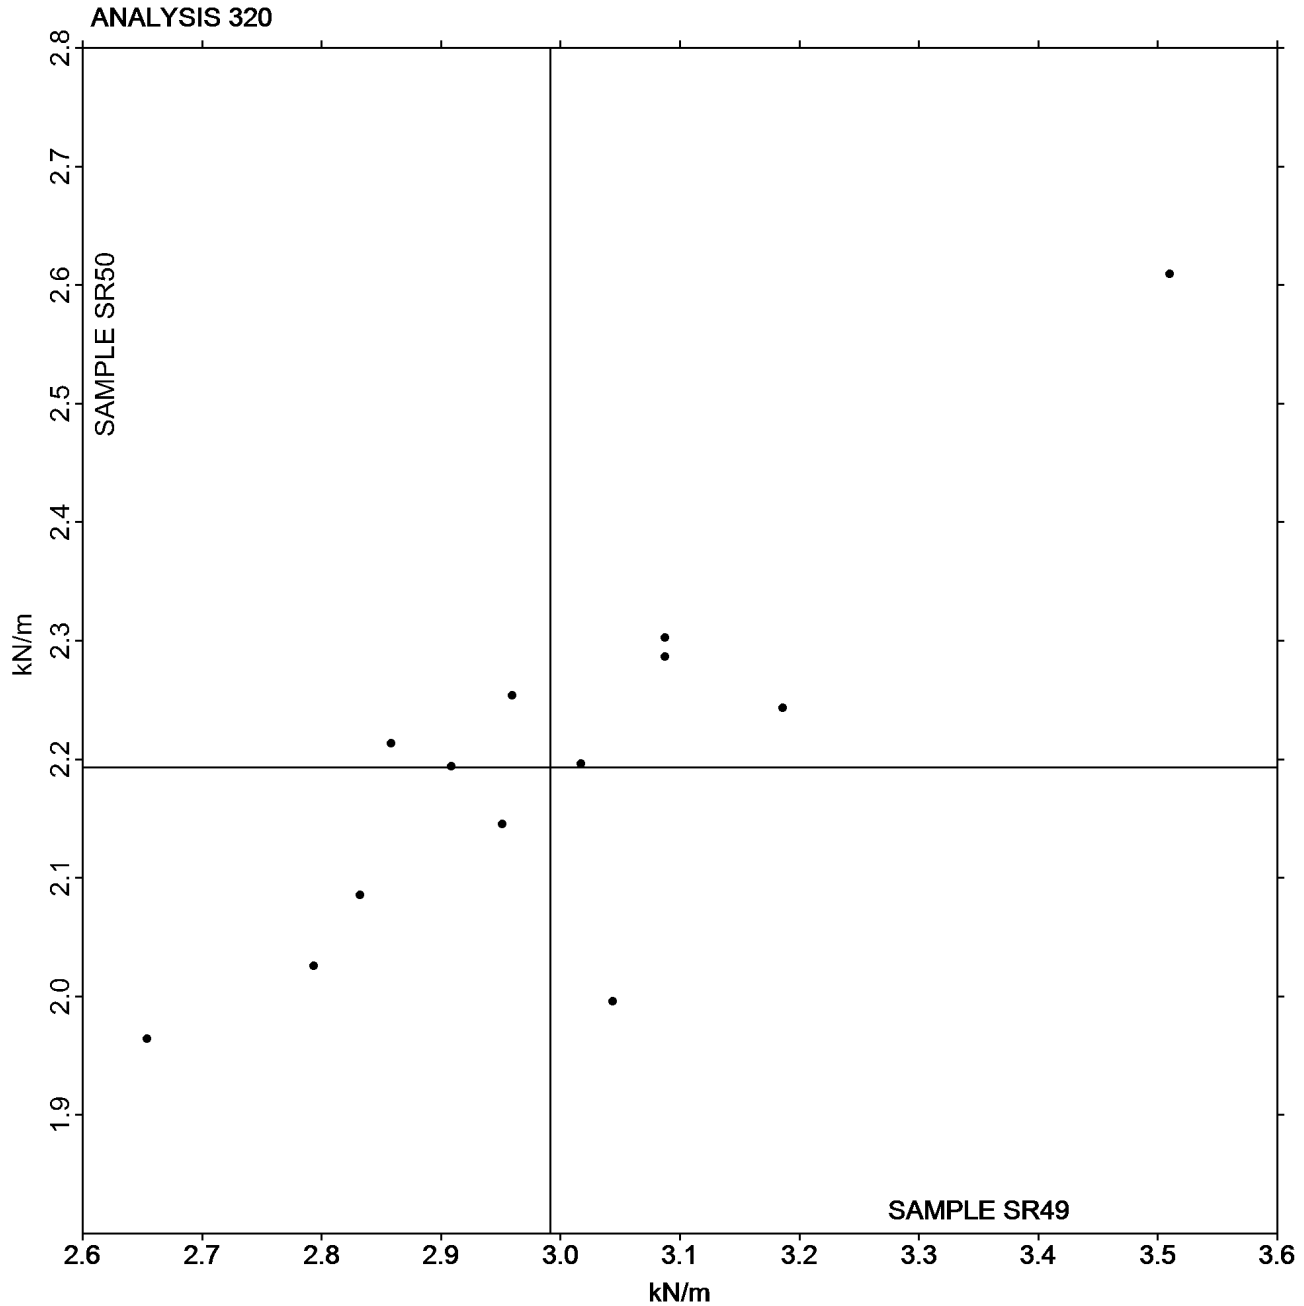

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 321
Tensile Energy Absorption - Newsprint
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SR49</u>			<u>Sample SR50</u>		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
76YQ6M		28.97	4.89	1.66	17.03	1.95	0.98
78HWMH		27.01	2.93	1.00	18.32	3.24	1.63
9JNN79		25.39	1.31	0.45	16.70	1.62	0.82
BWAKKC		22.90	-1.18	-0.40	15.36	0.28	0.14
DD7RR9		21.92	-2.16	-0.73	13.54	-1.54	-0.78
DMBWJP		27.73	3.65	1.24	16.96	1.89	0.95
JRMTN2		22.76	-1.33	-0.45	14.87	-0.20	-0.10
JVACU6		23.71	-0.37	-0.13	15.08	0.00	0.00
LP8D86		18.18	-5.90	-2.01	11.36	-3.72	-1.87
TQHKE7		25.01	0.93	0.32	14.67	-0.41	-0.21
XLUARC		22.54	-1.54	-0.52	12.66	-2.42	-1.22
Z38V2D		22.86	-1.22	-0.42	14.39	-0.69	-0.35

Summary Statistics	<u>Sample SR49</u>	<u>Sample SR50</u>
Grand Means	24.08 Joules/sq m	15.08 Joules/sq m
Stnd Dev Btwn Labs	2.94 Joules/sq m	1.98 Joules/sq m
Statistics based on 12 of 12 reporting participants.		



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 321


Tensile Energy Absorption - Newsprint

TAPPI Official Test Method T494

Grand Mean Sample SR49 = 24.081
Joules/sq m

Grand Mean Sample SR50 = 15.077
Joules/sq m

ANALYSIS 321

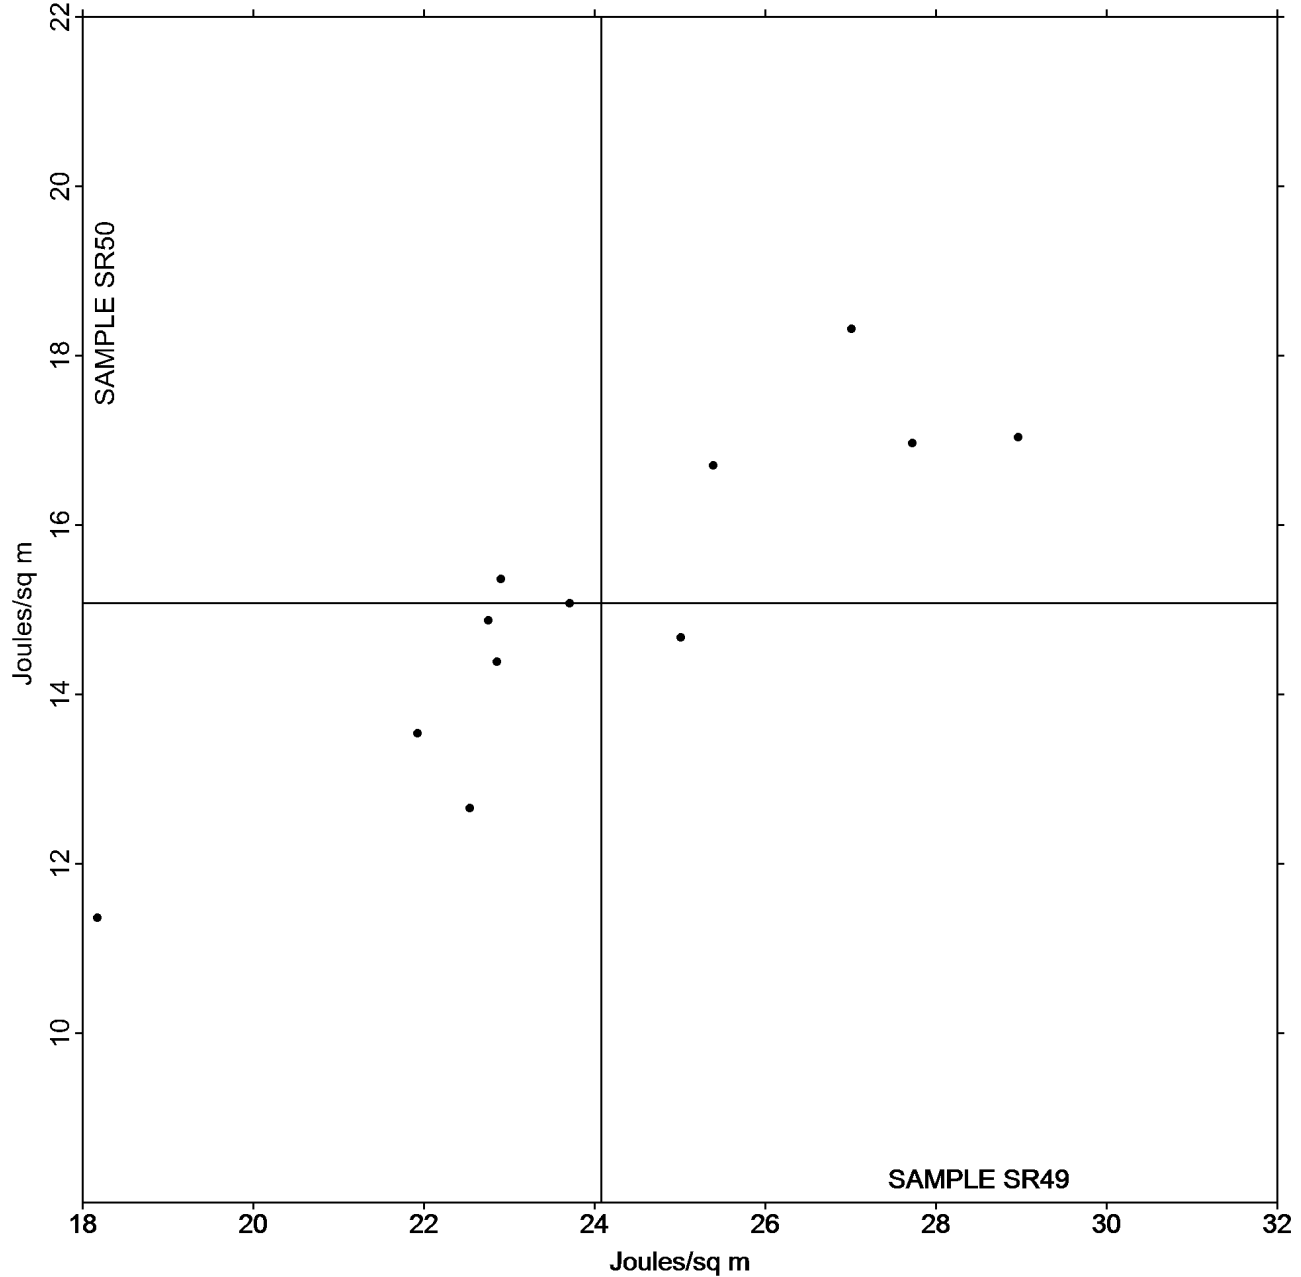

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 322
Elongation to Break - Newsprint
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SR49</u>			<u>Sample SR50</u>		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
76YQ6M		1.873	0.515	2.52	1.659	0.483	2.25
78HWMH		1.433	0.075	0.37	1.432	0.256	1.20
9JNN79		1.225	-0.133	-0.65	1.077	-0.099	-0.46
BWAKKC		1.275	-0.083	-0.40	1.135	-0.041	-0.19
DMBWJP		1.276	-0.082	-0.40	1.056	-0.120	-0.56
JRMTN2		1.249	-0.109	-0.53	1.123	-0.053	-0.25
JVACU6		1.508	0.150	0.73	1.330	0.154	0.72
LP8D86		1.102	-0.256	-1.25	0.905	-0.271	-1.26
TQHKE7		1.420	0.062	0.30	1.100	-0.076	-0.35
XLUARC		1.324	-0.034	-0.17	1.034	-0.142	-0.66
Z38V2D		1.251	-0.106	-0.52	1.085	-0.091	-0.42

Summary Statistics	<u>Sample SR49</u>	<u>Sample SR50</u>
Grand Means	1.36 Percent	1.18 Percent
Std Dev Btwn Labs	0.20 Percent	0.21 Percent

Statistics based on 11 of 11 reporting participants.




Paper & Paperboard Interlaboratory Testing Program
Analysis 322
Elongation to Break - Newsprint
TAPPI Official Test Method T494

Report #2911S,
November 2017

Grand Mean Sample SR49 = 1.3578
Percent

Grand Mean Sample SR50 = 1.1760
Percent

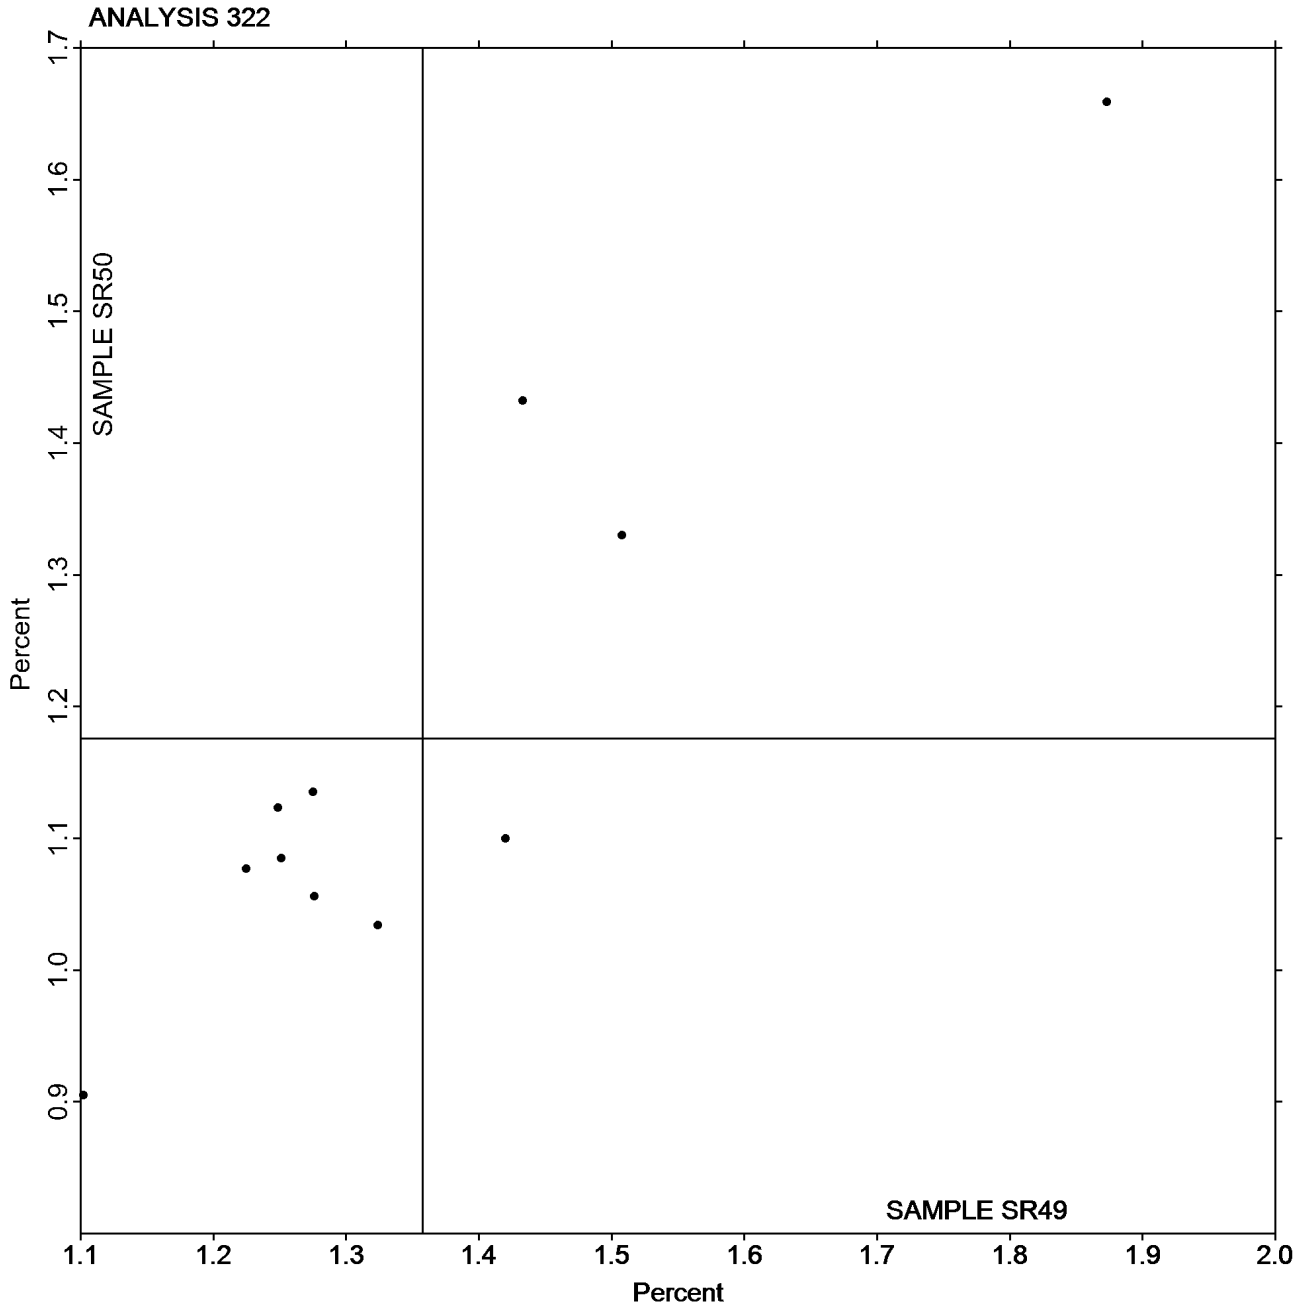

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program

**Report #2911S,
November 2017**

Analysis 325

Tensile Breaking Strength - Printing Papers

TAPPI Official Test Method T494

WebCode	Data Flag	Sample SF49			Sample SF50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
2E292A	X	3.661	-0.649	-2.97	3.751	-0.563	-2.47	CB
2G7Y4H		4.195	-0.114	-0.52	4.234	-0.080	-0.35	IM
2K76KA		4.404	0.094	0.43	4.284	-0.030	-0.13	LH
2V4BCM		4.045	-0.265	-1.21	4.058	-0.256	-1.12	IM
3GMFWQ		4.700	0.391	1.79	4.527	0.213	0.93	LA
3X9V39		4.163	-0.147	-0.67	4.222	-0.092	-0.40	LI
4AFC2N		4.611	0.301	1.38	4.629	0.315	1.38	TP
62XC6C		4.098	-0.212	-0.97	4.135	-0.179	-0.79	DL
778RCF	X	3.671	-0.639	-2.92	3.652	-0.662	-2.90	ID
7N7A2A		4.521	0.211	0.96	4.413	0.099	0.43	TP
7TPYPU		3.893	-0.417	-1.91	3.948	-0.366	-1.60	RE
7XXAUG		4.331	0.021	0.10	4.355	0.041	0.18	LX
874MCW		4.015	-0.294	-1.35	3.912	-0.403	-1.77	TB
883W7E		4.374	0.064	0.29	4.491	0.177	0.78	TC
92UQ72		4.575	0.266	1.21	4.519	0.205	0.90	LX
AHRGEG		4.583	0.273	1.25	4.647	0.333	1.46	TN
BJMDPW		4.087	-0.223	-1.02	4.034	-0.280	-1.23	LI
BNWNHQ		4.556	0.246	1.13	4.627	0.313	1.37	LI
CHGR3E		4.653	0.343	1.57	4.608	0.294	1.29	LA
CT3K2Q		4.557	0.247	1.13	4.587	0.273	1.20	LI
DJB NB9		4.301	-0.009	-0.04	4.378	0.064	0.28	LH
FLD4YQ		4.108	-0.201	-0.92	3.955	-0.360	-1.58	TS
FM7YJE		4.098	-0.212	-0.97	4.120	-0.195	-0.85	TB
FRFET3		4.073	-0.237	-1.08	4.145	-0.169	-0.74	TF
FZBE6A		4.228	-0.082	-0.37	4.207	-0.107	-0.47	XX
GZP2GW		4.303	-0.007	-0.03	4.220	-0.094	-0.41	XX
JRMTN2		4.103	-0.207	-0.95	4.170	-0.144	-0.63	LH
MDXUBV		4.232	-0.078	-0.36	4.251	-0.063	-0.27	TB
N3RAQE		4.237	-0.073	-0.33	4.316	0.002	0.01	LH
NBLFJF		4.190	-0.120	-0.55	4.036	-0.278	-1.22	TF
P4DMGV		4.475	0.165	0.76	4.527	0.213	0.93	TF
PP234X		4.298	-0.012	-0.05	4.405	0.091	0.40	LF
Q76ULT		4.049	-0.261	-1.19	4.104	-0.210	-0.92	LE
QC8Z3G		4.158	-0.152	-0.69	4.281	-0.033	-0.14	LI
QCBP6T		4.489	0.179	0.82	4.280	-0.034	-0.15	TJ
RPDFLR		3.959	-0.351	-1.60	3.808	-0.506	-2.22	LH
TVUHW2		4.342	0.032	0.15	4.377	0.063	0.28	LH
U46RAL		4.520	0.210	0.96	4.483	0.169	0.74	XX
UCX8W6		4.129	-0.180	-0.82	4.270	-0.044	-0.20	IM
VD46K7		4.567	0.257	1.18	4.680	0.366	1.60	LI



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 325

Tensile Breaking Strength - Printing Papers

TAPPI Official Test Method T494

WebCode	Data Flag	Sample SF49			Sample SF50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
WFAULU		4.316	0.006	0.03	4.341	0.027	0.12	LA
WFNFVV		4.394	0.084	0.38	4.465	0.151	0.66	TO
X93RPR		4.357	0.047	0.22	4.425	0.111	0.49	LA
XRYBPK	X	3.795	-0.515	-2.35	4.208	-0.106	-0.46	VM
ZMEABR		4.725	0.415	1.90	4.718	0.404	1.77	XX

Summary Statistics	Sample SF49	Sample SF50
Grand Means	4.31 kN/m	4.31 kN/m
Std Dev Btwn Labs	0.22 kN/m	0.23 kN/m

Statistics based on 42 of 45 reporting participants.

Comments on Assigned Data Flags for Test #325

778RCF (X) - Data for both samples are low. Possible Systematic Error.

XRYBPK (X) - Inconsistent in testing between samples. Inconsistent within the determinations of sample SF49.

2E292A (X) - Data for sample SF49 are low.

Key to Instrument Codes Reported by Participants

CB	Chatillon DFIS 50 (Digital Gauge)/TCD 200	DL	EMIC DL500 Universal Testing Machines
ID	Instron 4201/4202	IM	Instron 5500 Series
LA	L & W Tensile - Autoline 300	LE	L & W Tensile Tester 066
LF	L & W Tensile/Fracture Toughness Tester SE 064	LH	L & W Alwetron TH1 (Horizontal) SE 060/065F
LI	L & W Tensile Tester SE 062	LX	L & W (model not specified)
RE	Regmed	TB	Thwing-Albert EJA/1000
TC	Thwing-Albert Electro-Hydraulic, Model 30LT	TF	Thwing-Albert EJA Vantage-1
TJ	Thwing-Albert QC II-XS	TN	Testometric M100-1CT
TO	Thwing-Albert QC-1000	TP	TMI Monitor/Tensile 100 (84-21-01)
TS	Tinius Olsen 1000	VM	Valmet PaperLab (was Kajaani/Robotest)
XX	Instrument make/model not specified by lab		



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 325


Tensile Breaking Strength - Printing Papers

TAPPI Official Test Method T494

Grand Mean Sample SF49 = 4.3098
kN/m

Grand Mean Sample SF50 = 4.3141
kN/m

ANALYSIS 325

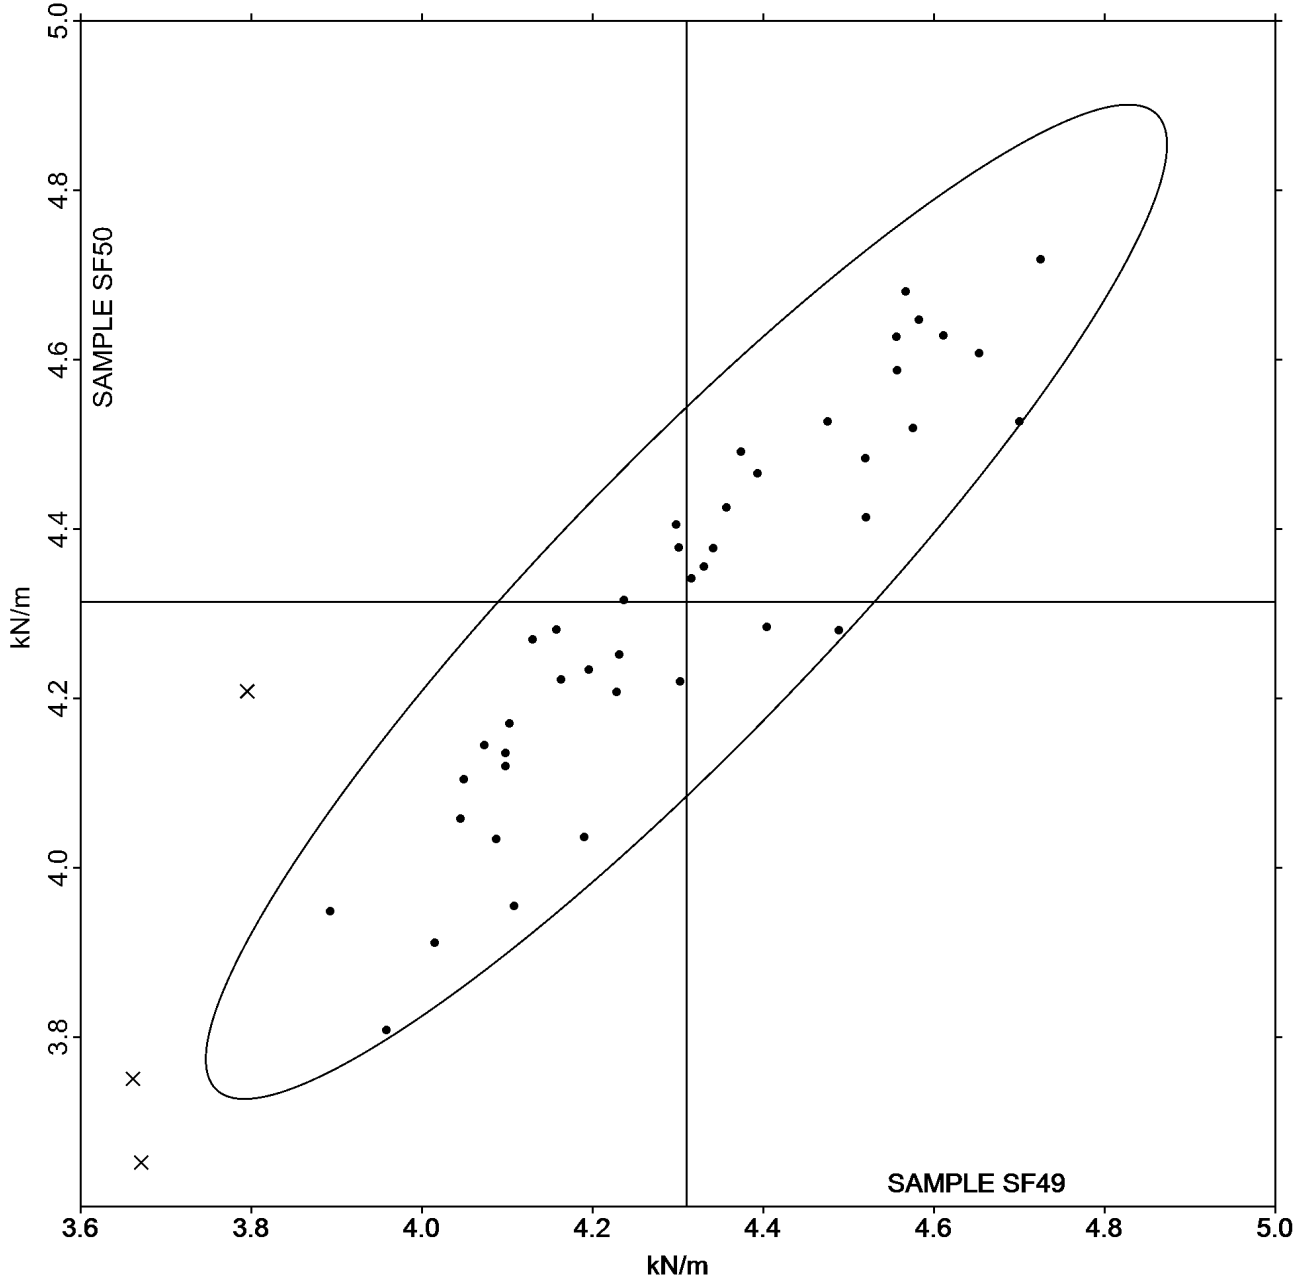



Paper & Paperboard Interlaboratory Testing Program

**Report #2911S,
November 2017**

Analysis 327

Tensile Energy Absorption - Printing Papers

TAPPI Official Test Method T494

WebCode	Data Flag	Sample SF49			Sample SF50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
2G7Y4H		43.12	-0.38	-0.08	46.07	1.33	0.25	IM
2K76KA		47.78	4.27	0.89	46.99	2.25	0.43	LH
2V4BCM		48.09	4.59	0.95	49.55	4.81	0.92	IM
3GMFWQ		51.47	7.96	1.65	53.74	9.00	1.72	LA
3X9V39		38.86	-4.64	-0.96	42.62	-2.12	-0.41	LI
62XC6C		44.65	1.15	0.24	44.28	-0.46	-0.09	DL
778RCF		46.76	3.26	0.67	46.23	1.49	0.29	ID
7TPYPU		38.74	-4.76	-0.99	40.23	-4.51	-0.86	RE
7XXAUG		40.98	-2.52	-0.52	43.01	-1.73	-0.33	LX
92UQ72		47.93	4.42	0.92	47.57	2.83	0.54	LX
AHRGEG		47.92	4.42	0.92	48.98	4.24	0.81	LX
BJMDPW		40.15	-3.36	-0.70	39.90	-4.85	-0.93	LI
BNWNHQ		48.74	5.24	1.08	54.14	9.40	1.80	LI
CT3K2Q		47.25	3.74	0.78	48.97	4.23	0.81	LI
DJB9B9		42.61	-0.89	-0.19	43.20	-1.54	-0.30	LH
FM7YJE		44.45	0.94	0.20	45.22	0.48	0.09	TB
FZBE6A		36.09	-7.41	-1.54	33.11	-11.63	-2.23	XX
GZP2GW		49.74	6.24	1.29	53.40	8.66	1.66	XX
JRMTN2		40.29	-3.22	-0.67	41.18	-3.56	-0.68	LH
MDXUBV		43.92	0.42	0.09	43.99	-0.75	-0.14	TB
N3RAQE		43.83	0.32	0.07	43.97	-0.77	-0.15	LH
NBLFJF		47.95	4.45	0.92	45.41	0.67	0.13	TF
P4DMGV		47.65	4.15	0.86	48.60	3.86	0.74	TF
PP234X		34.16	-9.34	-1.93	37.91	-6.83	-1.31	LW
QC8Z3G		40.62	-2.88	-0.60	43.90	-0.84	-0.16	LI
RPDFLR		38.29	-5.21	-1.08	37.32	-7.42	-1.42	LH
UCX8W6		41.39	-2.11	-0.44	46.85	2.11	0.40	IM
VD46K7		47.86	4.35	0.90	48.80	4.06	0.78	LI
WFAULU		32.05	-11.45	-2.37	32.66	-12.08	-2.31	LA
WFNFVV		39.48	-4.03	-0.83	42.44	-2.30	-0.44	TO
X93RPR		45.78	2.28	0.47	46.70	1.96	0.38	LA

Summary Statistics	Sample SF49	Sample SF50
Grand Means	43.50 Joules/sq m	44.74 Joules/sq m
Std Dev Btwn Labs	4.83 Joules/sq m	5.22 Joules/sq m
Statistics based on 31 of 31 reporting participants.		

Comments on Assigned Data Flags for Test #327



Paper & Paperboard Interlaboratory Testing Program
Analysis 327
Tensile Energy Absorption - Printing Papers
TAPPI Official Test Method T494

Report #2911S,
November 2017

Analysis Notes:

778RCF - Data appears to be off by a factor of 10. Data corrected by CTS.

MDXUBV - Data appear to be reported as kg-m/sq m, not J/sq m as indicated on datasheet. Units corrected by CTS.

Key to Instrument Codes Reported by Participants

DL	EMIC DL500 Universal Testing Machines	ID	Instron 4201
IM	Instron 5500 Series	LA	L & W Tensile - Autoline 300
LH	L & W Alwetron TH1 (Horizontal) SE 060	LI	L & W Tensile Tester SE 062
LW	L & W Tensile Tester SE 064	LX	L & W (model not specified)
RE	Regmed	TB	Thwing-Albert EJA/1000
TF	Thwing-Albert EJA Vantage-1	TO	Thwing-Albert QC-1000
XX	Instrument make/model not specified by lab		



Analysis 327


Tensile Energy Absorption - Printing Papers

TAPPI Official Test Method T494

Grand Mean Sample SF49 = 43.503
Joules/sq m

Grand Mean Sample SF50 = 44.740
Joules/sq m

ANALYSIS 327

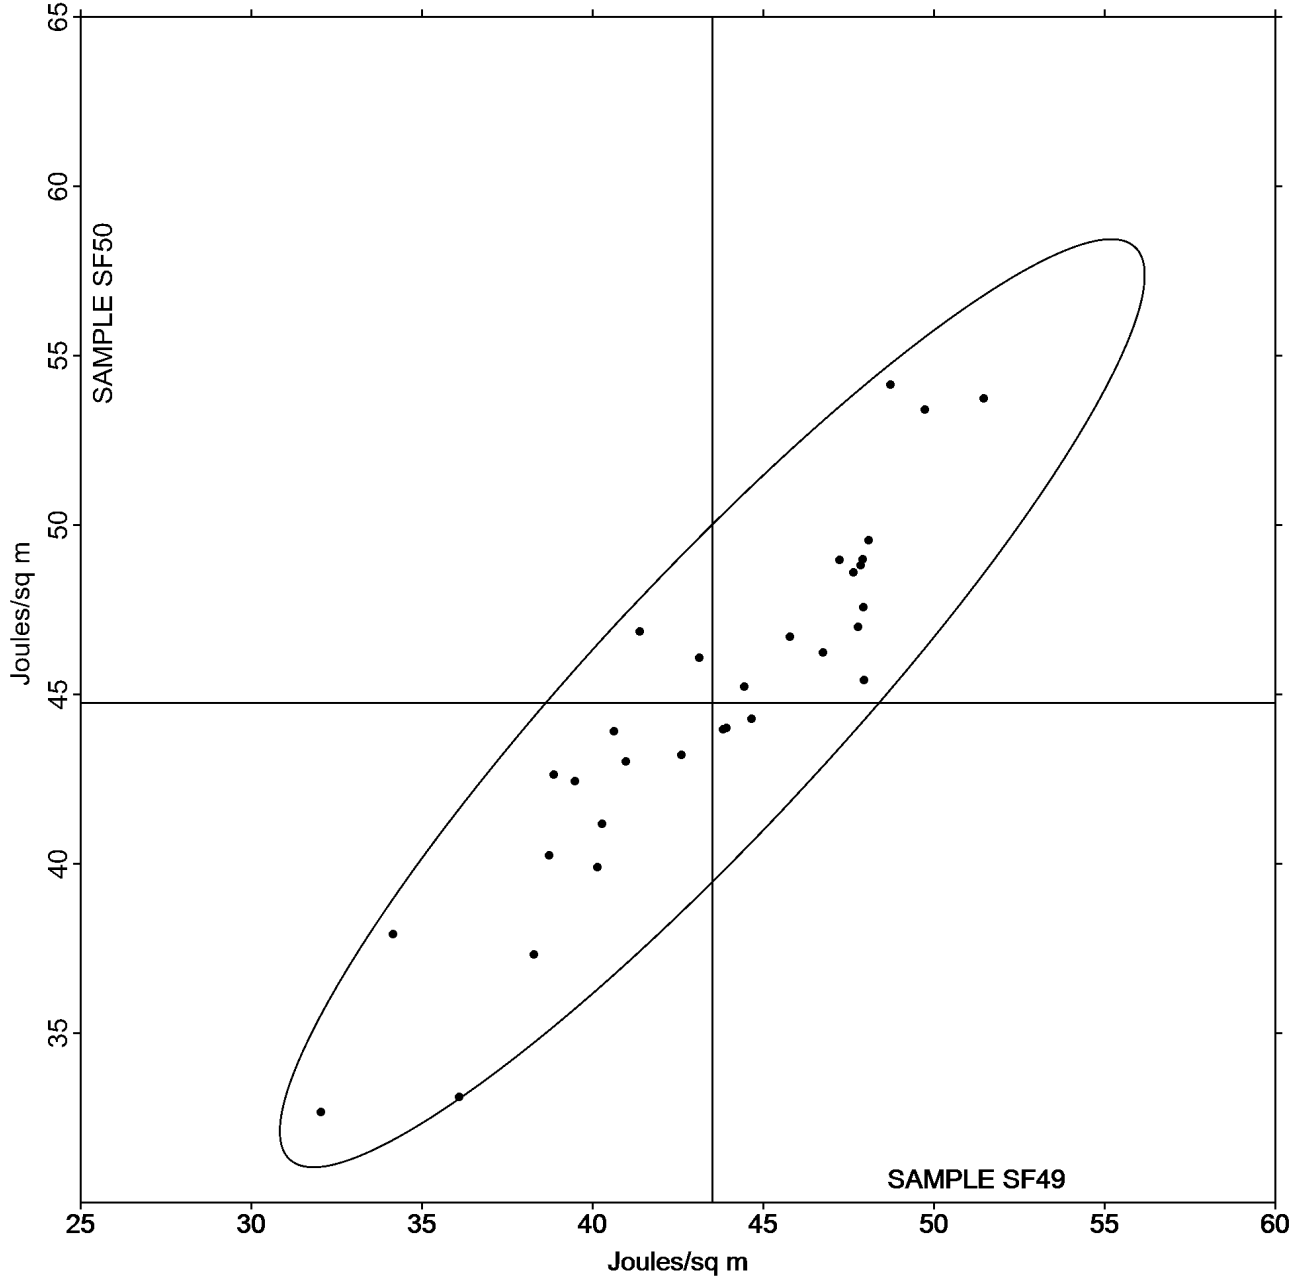



Paper & Paperboard Interlaboratory Testing Program
Analysis 328
Elongation to Break - Printing Papers
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	Sample SF49			Sample SF50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
2G7Y4H		1.619	0.052	0.34	1.707	0.105	0.82	IM
2K76KA		1.642	0.075	0.50	1.665	0.063	0.49	LH
2V4BCM	X	2.011	0.444	2.92	2.039	0.437	3.40	XX
3GMFWQ		1.533	-0.034	-0.22	1.649	0.047	0.37	LA
3X9V39		1.456	-0.111	-0.73	1.565	-0.037	-0.28	LI
62XC6C		1.771	0.204	1.35	1.763	0.161	1.25	DL
778RCF		1.753	0.187	1.23	1.730	0.128	1.00	ID
7TPYPU		1.650	0.083	0.55	1.648	0.047	0.36	RE
7XXAUG		1.453	-0.114	-0.75	1.506	-0.096	-0.74	LX
874MCW		1.422	-0.145	-0.95	1.469	-0.133	-1.03	TF
92UQ72		1.588	0.021	0.14	1.629	0.027	0.21	LX
AHRGEG		1.510	-0.057	-0.37	1.507	-0.095	-0.73	LX
BJMDPW		1.497	-0.070	-0.46	1.512	-0.090	-0.70	LI
BNWNHQ	*	1.652	0.085	0.56	1.792	0.190	1.48	LI
CT3K2Q		1.592	0.025	0.17	1.644	0.042	0.33	LI
DJB9B		1.499	-0.068	-0.44	1.524	-0.078	-0.60	LH
FLD4YQ	X	0.128	-1.438	-9.46	0.122	-1.479	-11.49	TS
FM7YJE		1.688	0.122	0.80	1.706	0.105	0.81	TB
FRFET3		1.720	0.153	1.01	1.690	0.088	0.69	TF
FZBE6A		1.742	0.175	1.15	1.639	0.037	0.29	XX
GZP2GW		1.764	0.197	1.30	1.790	0.188	1.46	XX
JRMTN2		1.513	-0.054	-0.35	1.521	-0.081	-0.63	LH
MDXUBV		1.613	0.046	0.30	1.604	0.003	0.02	TB
N3RAQE		1.610	0.043	0.29	1.604	0.002	0.02	LH
NBLFJF		1.837	0.271	1.78	1.802	0.201	1.56	TF
P4DMGV		1.811	0.244	1.61	1.835	0.233	1.81	TF
PP234X		1.289	-0.278	-1.83	1.380	-0.222	-1.72	LX
QC8Z3G		1.504	-0.063	-0.41	1.573	-0.029	-0.22	LI
RPDFLR		1.484	-0.083	-0.54	1.478	-0.124	-0.96	LH
UCX8W6		1.563	-0.004	-0.02	1.696	0.094	0.73	IM
VD46K7		1.515	-0.052	-0.34	1.544	-0.058	-0.45	LI
WFAULU		1.416	-0.151	-0.99	1.443	-0.159	-1.23	LA
WFNFVV		1.358	-0.209	-1.37	1.432	-0.170	-1.32	TG
X93RPR		1.472	-0.095	-0.62	1.473	-0.129	-1.00	XX
XRYBPK	*	1.160	-0.407	-2.68	1.330	-0.272	-2.11	VM



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 328

Elongation to Break - Printing Papers

TAPPI Official Test Method T494

Summary Statistics	Sample SF49	Sample SF50
Grand Means	1.57 Percent	1.60 Percent
Std Dev Btwn Labs	0.15 Percent	0.13 Percent

Statistics based on 33 of 35 reporting participants.

Comments on Assigned Data Flags for Test #328

2V4BCM (X) - Data for both samples are high. Possible Systematic Error.

FLD4YQ (X) - Extreme Data.

Key to Instrument Codes Reported by Participants

DL	EMIC DL500 Universal Testing Machines	ID	Instron 4201
IM	Instron 5500	LA	L & W Tensile - Autoline 300
LH	L & W Alwetron TH1 (Horizontal) SE 060	LI	L & W Tensile Tester SE 062
LX	L & W (model not specified)	RE	Regmed
TB	Thwing-Albert EJA/1000	TF	Thwing-Albert EJA Vantage-1
TG	Thwing-Albert QC	TS	Tinius Olsen 1000
VM	Valmet PaperLab (was Kajaani/Robotest)	XX	Instrument make/model not specified by lab



Paper & Paperboard Interlaboratory Testing Program


Report #2911S,
November 2017

Analysis 328 Elongation to Break - Printing Papers TAPPI Official Test Method T494

Grand Mean Sample SF49 = 1.5666
Percent

Grand Mean Sample SF50 = 1.6016
Percent

ANALYSIS 328

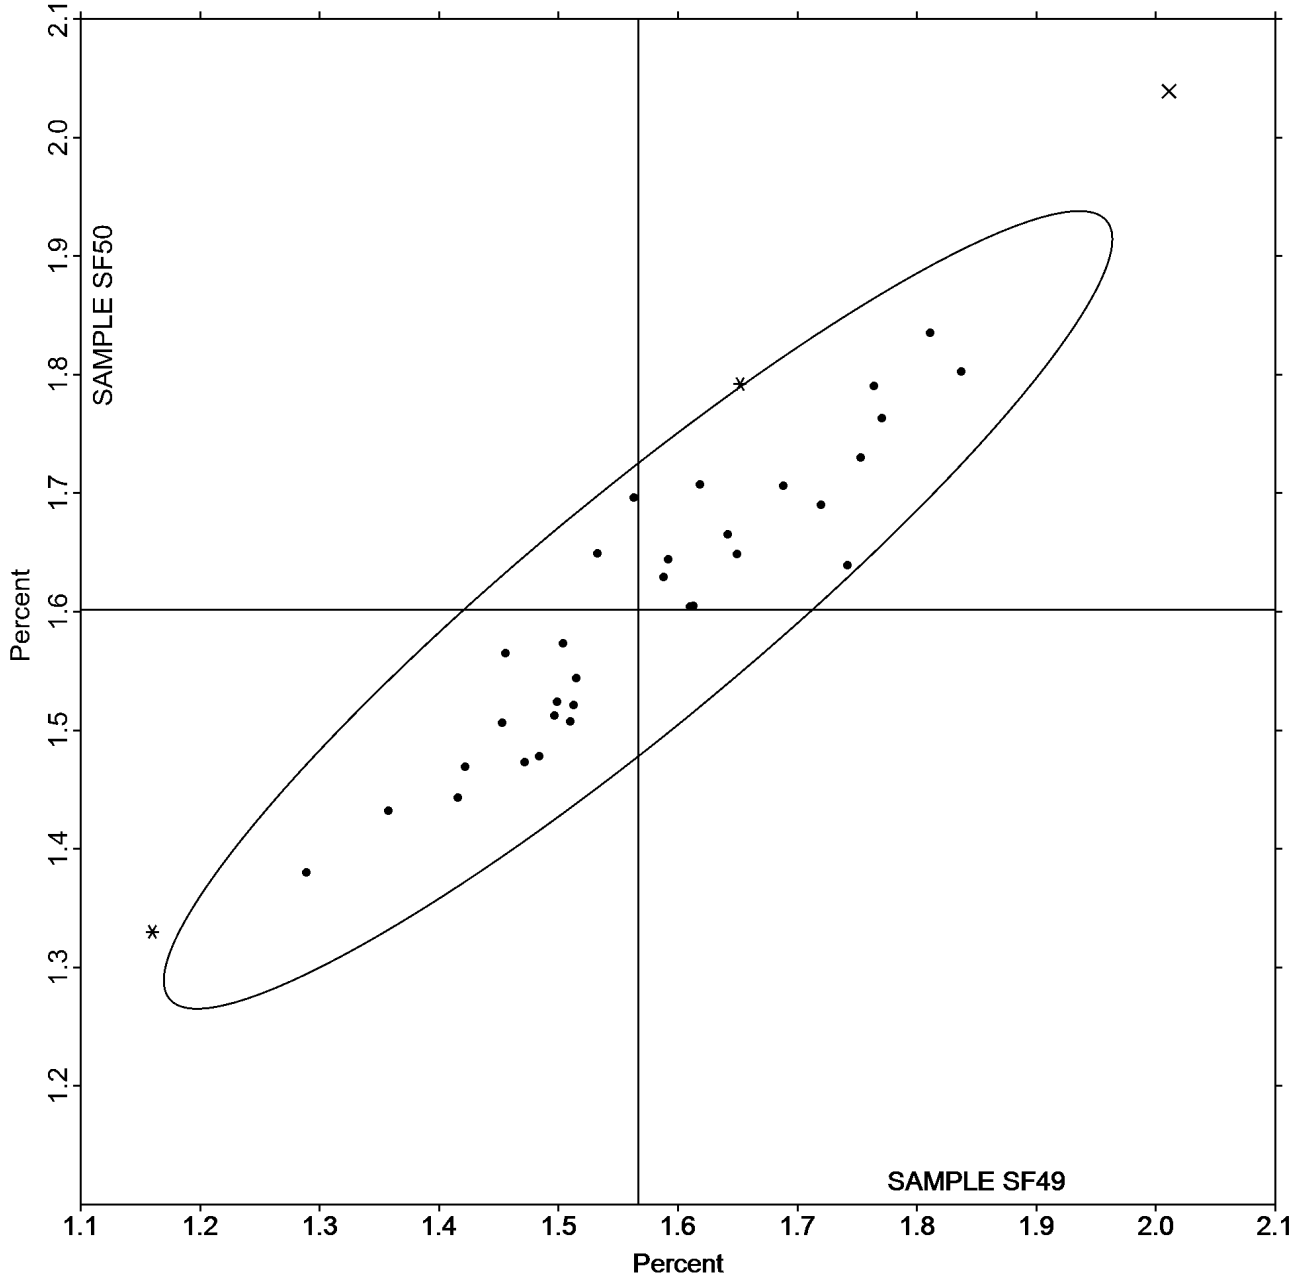



Paper & Paperboard Interlaboratory Testing Program

**Report #2911S,
November 2017**

Analysis 330

Tensile Breaking Strength - Packaging Papers

TAPPI Official Test Method T494

WebCode	Data Flag	Sample SE49			Sample SE50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
6MK47U		16.11	-0.29	-0.30	13.16	0.33	0.38	LI
7YQGZY		17.56	1.16	1.23	13.15	0.32	0.38	TR
882X9Y		18.56	2.16	2.28	14.75	1.92	2.26	LA
8NK38C		16.31	-0.08	-0.09	12.79	-0.05	-0.05	TB
96M2TK		14.92	-1.48	-1.56	11.23	-1.60	-1.88	IN
99RMQJ		15.93	-0.47	-0.49	12.48	-0.35	-0.41	LE
9FAQZ8		16.55	0.15	0.16	12.46	-0.37	-0.43	ID
B7VM6R		16.93	0.53	0.56	13.74	0.91	1.07	TO
BW9TNP		15.30	-1.09	-1.16	11.80	-1.03	-1.22	LE
C7BE89	*	18.54	2.14	2.26	13.76	0.92	1.09	IK
D6TVM3		17.72	1.32	1.39	13.71	0.88	1.03	LX
DJDDGR		17.20	0.81	0.85	13.15	0.32	0.38	XX
E7YPV8		17.45	1.05	1.11	13.98	1.15	1.35	TX
EQB6LE		15.00	-1.40	-1.48	12.09	-0.74	-0.87	TB
FEU3E8		15.85	-0.54	-0.57	12.16	-0.67	-0.78	LE
FLALWL		16.42	0.02	0.03	12.90	0.07	0.09	LH
FMAGLJ		15.53	-0.87	-0.92	12.16	-0.67	-0.78	TH
GAWZRJ		15.64	-0.76	-0.80	12.05	-0.79	-0.92	IF
GL7FVH		16.37	-0.03	-0.03	12.06	-0.77	-0.91	XX
GQGJWD	X	13.56	-2.84	-3.00	9.97	-2.86	-3.37	ID
MDXUBV		16.10	-0.29	-0.31	12.94	0.11	0.13	TB
MDXVDG		14.47	-1.93	-2.04	10.96	-1.87	-2.20	TT
MGUPN4		17.89	1.50	1.58	13.99	1.15	1.36	TH
MYDGVF		16.97	0.57	0.61	13.69	0.86	1.01	TO
N3RAQE		16.05	-0.35	-0.37	12.51	-0.32	-0.38	LH
NH338Q		16.00	-0.40	-0.42	12.71	-0.12	-0.15	XX
P4DMGV	*	15.75	-0.65	-0.69	13.65	0.82	0.96	TO
Q2BXZ9		14.82	-1.58	-1.67	11.59	-1.24	-1.46	TO
QTX3JK		16.08	-0.32	-0.34	12.21	-0.62	-0.74	IF
QUAHDL		17.02	0.62	0.66	13.42	0.59	0.69	LE
QVKMNP		15.53	-0.86	-0.91	12.51	-0.32	-0.38	IF
RDLP49		16.56	0.17	0.18	13.27	0.44	0.51	ID
T8PHX6		17.42	1.02	1.08	14.52	1.69	1.99	LA
T8PM98		15.94	-0.45	-0.48	12.13	-0.70	-0.83	IM
TG8BYZ	X	13.73	-2.67	-2.82	12.23	-0.60	-0.71	IM
UGR6LV		16.19	-0.20	-0.22	12.81	-0.02	-0.02	LA
UQHPP9		15.31	-1.09	-1.15	12.14	-0.69	-0.81	XX
VA4Y2U		17.43	1.03	1.09	13.31	0.48	0.56	LW
VT3WPV		17.30	0.90	0.95	13.03	0.20	0.24	LH
W8DWW7		15.78	-0.62	-0.65	12.13	-0.70	-0.83	IM



Paper & Paperboard Interlaboratory Testing Program
Analysis 330
Tensile Breaking Strength - Packaging Papers
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SE49</u>			<u>Sample SE50</u>			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
WLVUTU		16.36	-0.04	-0.04	12.90	0.07	0.08	TA
XQP2XN		16.14	-0.26	-0.27	12.14	-0.69	-0.81	LE
XUNH9W		16.80	0.40	0.42	12.32	-0.52	-0.61	LW
XX7LWU		17.27	0.87	0.92	14.19	1.36	1.60	TH
Y46LT2		15.51	-0.89	-0.94	12.22	-0.61	-0.72	TK
Y4A4V7		17.00	0.61	0.64	13.80	0.97	1.14	TH
ZXY8NB		16.30	-0.10	-0.10	12.74	-0.09	-0.11	IK

Summary Statistics	<u>Sample SE49</u>	<u>Sample SE50</u>
Grand Means	16.40 kN/m	12.83 kN/m
Std Dev Btwn Labs	0.95 kN/m	0.85 kN/m

Statistics based on 45 of 47 reporting participants.

Comments on Assigned Data Flags for Test #330

GQGJWD (X) - Data for both samples are low. Possible Systematic Error. Inconsistent within the determinations of both samples.

TG8BYZ (X) - Data for sample SE49 are low. Inconsistent within the determinations of sample SE49.

Key to Instrument Codes Reported by Participants

ID	Instron 4201	IF	Instron 3340 Series
IK	Instron 4400 Series	IM	Instron 5500 Series
IN	Instron 3360 Series	LA	L & W Autoline
LE	L & W Tensile Tester 066	LH	L & W Alwetron TH1 (Horizontal) SE 060
LI	Lloyds Instruments	LW	L & W Tensile Tester SE062
LX	L & W (model not specified)	TA	Thwing-Albert Tensile Tester
TB	Thwing-Albert EJA/1000	TH	Thwing-Albert QC-3A
TK	Thwing-Albert Model 37-4	TO	Thwing-Albert QC-1000
TR	TMI Horizontal Tensile Tester	TT	Tinius Olsen Model MHT
TX	Thwing-Albert (model not specified)	XX	Instrument make/model not specified by lab



Paper & Paperboard Interlaboratory Testing Program

**Report #2911S,
November 2017**

Analysis 331

Tensile Energy Absorption - Packaging Papers

TAPPI Official Test Method T494

WebCode	Data Flag	Sample SE49			Sample SE50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
7YQGZY		213.9	26.6	1.56	175.7	6.5	0.35	TR
882X9Y		193.8	6.5	0.38	178.6	9.4	0.51	LA
8NK38C		202.1	14.8	0.87	177.6	8.4	0.46	TB
96M2TK	*	187.9	0.6	0.03	132.2	-37.0	-2.02	IN
99RMQJ		175.5	-11.8	-0.70	156.2	-13.0	-0.71	LE
9FAQZ8	*	170.2	-17.1	-1.00	198.2	29.0	1.58	ID
B7VM6R		217.7	30.4	1.78	193.4	24.2	1.32	TO
BW9TNP		168.4	-18.9	-1.11	152.3	-16.9	-0.92	LE
C7BE89	X	197.7	10.4	0.61	124.6	-44.6	-2.43	XX
D6TVM3		203.3	15.9	0.94	180.6	11.4	0.62	LX
DJDDGR		201.2	13.9	0.81	152.7	-16.5	-0.90	XX
E7YPV8		215.4	28.0	1.65	202.5	33.3	1.82	XX
FEU3E8		173.4	-14.0	-0.82	160.2	-9.0	-0.49	LE
FLALWL		168.5	-18.9	-1.11	161.7	-7.5	-0.41	LH
FMAGLJ		206.9	19.6	1.15	185.2	16.0	0.87	TH
GL7FVH		183.7	-3.6	-0.21	150.1	-19.1	-1.04	XX
GQGJWD	X	111.6	-75.8	-4.45	85.6	-83.6	-4.56	ID
MDXUBV		169.0	-18.4	-1.08	167.7	-1.5	-0.08	TB
MDXVDG	X	250.1	62.7	3.68	188.5	19.3	1.05	TT
MGUPN4		214.1	26.7	1.57	193.7	24.5	1.34	TH
MYDGVF		190.7	3.4	0.20	182.2	13.0	0.71	TO
N3RAQE		175.8	-11.5	-0.68	159.9	-9.3	-0.51	LH
NH338Q	X	254.8	67.5	3.96	236.1	66.9	3.65	XX
P4DMGV		184.6	-2.7	-0.16	176.9	7.7	0.42	TO
Q2BXZ9		190.7	3.4	0.20	170.2	1.0	0.05	TO
QTX3JK		208.5	21.2	1.24	200.0	30.8	1.68	IF
QUAHDL		202.4	15.1	0.88	181.6	12.4	0.68	LE
QVKMNP		181.7	-5.7	-0.33	156.4	-12.8	-0.70	IN
T8PHX6		195.0	7.6	0.45	177.7	8.5	0.46	LA
T8PM98		186.6	-0.7	-0.04	153.6	-15.6	-0.85	IM
TG8BYZ		163.7	-23.7	-1.39	161.4	-7.8	-0.43	IM
UGR6LV		176.5	-10.8	-0.63	174.9	5.7	0.31	LA
UQHPP9	X	312.6	125.3	7.36	281.8	112.6	6.14	XX
VA4Y2U		174.0	-13.3	-0.78	153.9	-15.3	-0.84	LW
VT3WPV		165.9	-21.4	-1.26	151.3	-17.9	-0.97	LH
W8DWW7		171.9	-15.4	-0.91	158.6	-10.6	-0.58	IM
WLVUTU		169.0	-18.3	-1.08	147.8	-21.4	-1.17	TA
XQP2XN		169.3	-18.0	-1.06	146.3	-22.9	-1.25	LE
XUNH9W		167.0	-20.3	-1.19	142.4	-26.8	-1.46	LW
XX7LWU		198.4	11.1	0.65	201.3	32.1	1.75	TH



Paper & Paperboard Interlaboratory Testing Program

**Report #2911S,
November 2017**

Analysis 331

Tensile Energy Absorption - Packaging Papers

TAPPI Official Test Method T494

WebCode	Data Flag	Sample SE49			Sample SE50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
Y46LT2		179.3	-8.0	-0.47	159.2	-10.0	-0.55	TK
ZXY8NB		215.4	28.1	1.65	186.1	16.9	0.92	IK

Summary Statistics	Sample SE49	Sample SE50
Grand Means	187.34 Joules/sq m	169.20 Joules/sq m
Std Dev Btwn Labs	17.03 Joules/sq m	18.33 Joules/sq m
Statistics based on 37 of 42 reporting participants.		

Comments on Assigned Data Flags for Test #331

UQHPP9 (X) - Extreme Data.

MDXVDG (X) - Data for sample SE49 are high.

C7BE89 (X) - Inconsistent in testing between samples.

GQGJWD (X) - Data for both samples are low. Inconsistent within the determinations of sample SE49.

NH338Q (X) - Data for both samples are high.

Analysis Notes:

DJDDGR - Data appear to be reported as J/sq m, not ft-lb/sq ft inch as indicated on datasheet. Units corrected by CTS.

E7YPV8 - Data appear to be reported as ft-lb/sq ft, not inch-lb/sq inch as indicated on datasheet. Units corrected by CTS.

Key to Instrument Codes Reported by Participants

ID	Instron 4201	IF	Instron 3340 Series
IK	Instron 4400 Series	IM	Instron 5500 Series
IN	Instron 3360 Series	LA	L & W Autoline
LE	L & W Tensile Tester 066	LH	L & W Alwetron TH1 (Horizontal) SE 060
LW	L & W Tensile Tester SE062	LX	L & W (model not specified)
TA	Thwing-Albert Tensile Tester	TB	Thwing-Albert EJA/1000
TH	Thwing-Albert QC-3A	TK	Thwing-Albert Model 37-4
TO	Thwing-Albert QC-1000	TR	TMI Horizontal Tensile Tester
TT	Tinius Olsen Model MHT	XX	Instrument make/model not specified by lab



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 331


Tensile Energy Absorption - Packaging Papers

TAPPI Official Test Method T494

Grand Mean Sample SE49 = 187.34
Joules/sq m

Grand Mean Sample SE50 = 169.20
Joules/sq m

ANALYSIS 331

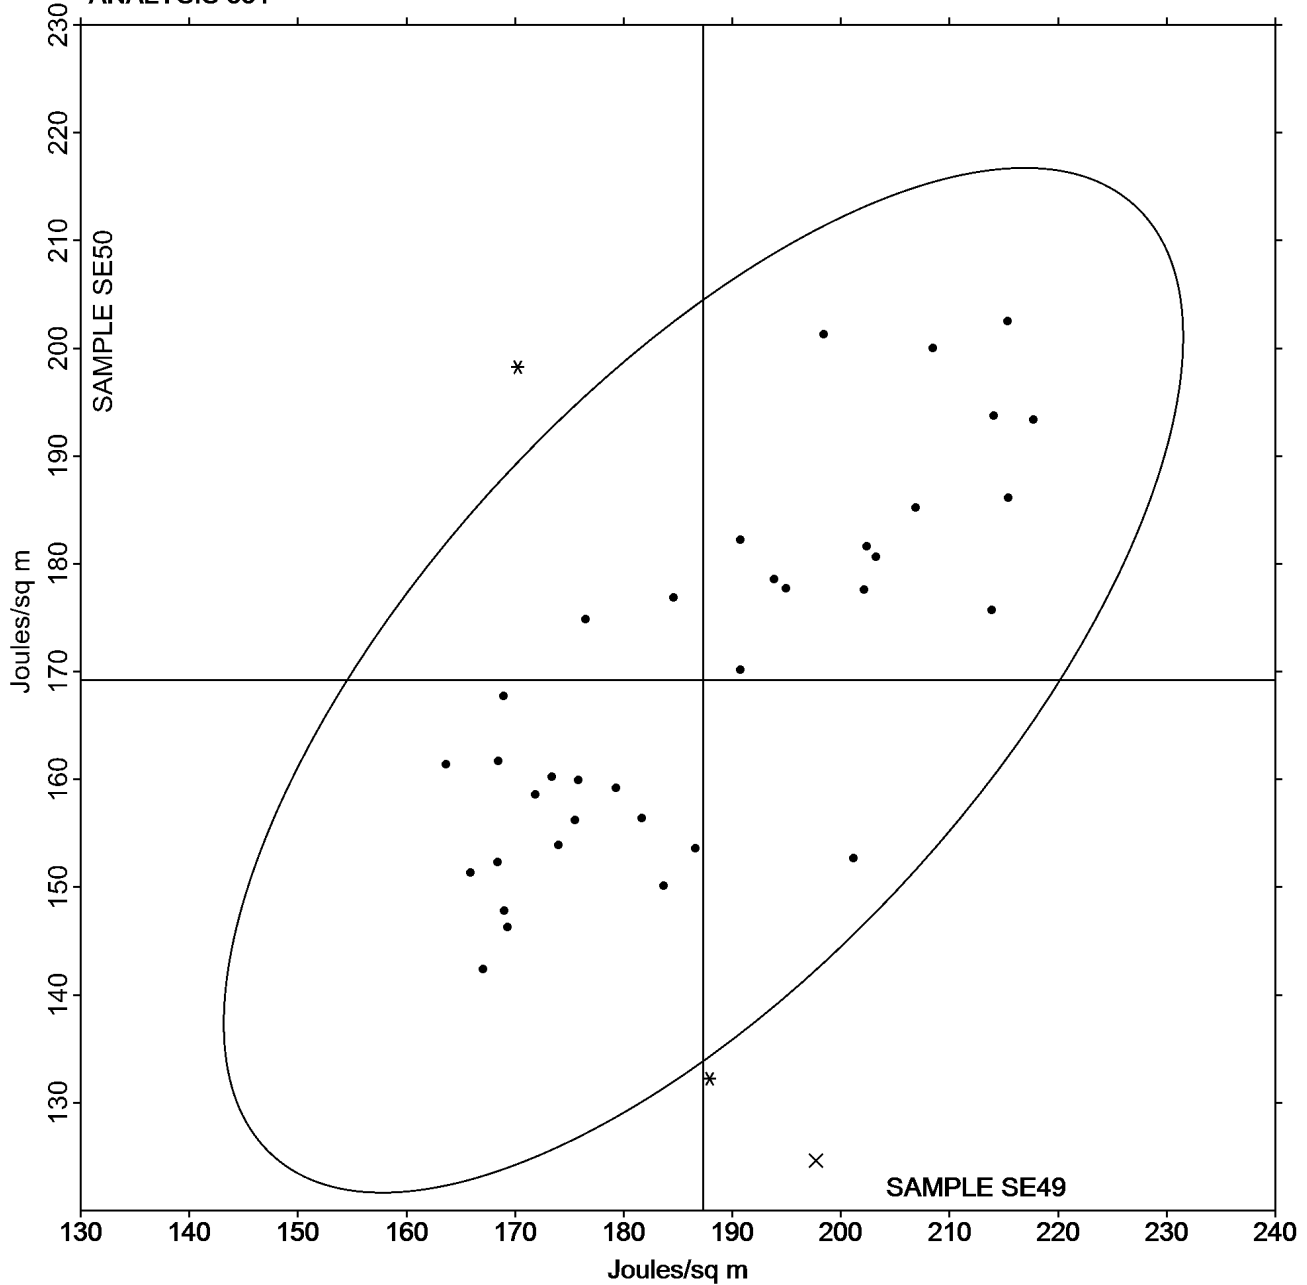



Paper & Paperboard Interlaboratory Testing Program
Analysis 332
Elongation to Break - Packaging Papers
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	Sample SE49			Sample SE50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
7YQGZY		1.924	0.134	0.57	2.148	0.075	0.32	TR
882X9Y		1.531	-0.260	-1.11	1.828	-0.245	-1.04	LA
8NK38C		1.950	0.159	0.68	2.220	0.147	0.62	TB
96M2TK	X	2.160	0.369	1.58	2.080	0.007	0.03	IN
99RMQJ		1.649	-0.142	-0.61	1.904	-0.169	-0.72	LE
9FAQZ8		1.846	0.056	0.24	2.117	0.044	0.19	ID
B7VM6R		2.128	0.337	1.45	2.330	0.257	1.09	TO
BW9TNP		1.652	-0.139	-0.59	1.977	-0.096	-0.41	LE
C7BE89	X	1.995	0.204	0.88	1.825	-0.248	-1.05	XX
D6TVM3		1.714	-0.077	-0.33	1.999	-0.074	-0.31	LX
DJDDGR	*	2.195	0.404	1.73	2.216	0.143	0.61	XX
E7YPV8		2.100	0.309	1.33	2.441	0.368	1.56	XX
EQB6LE		1.442	-0.349	-1.50	1.837	-0.235	-1.00	TB
FEU3E8		1.613	-0.178	-0.76	1.972	-0.101	-0.43	LE
FLALWL		1.568	-0.223	-0.95	1.925	-0.148	-0.63	LH
FMAGLJ		2.243	0.452	1.94	2.567	0.494	2.09	TH
GL7FVH		1.703	-0.088	-0.38	1.912	-0.161	-0.68	XX
GQGJWD		1.542	-0.249	-1.07	1.644	-0.429	-1.82	ID
MDXUBV		1.628	-0.162	-0.70	1.992	-0.081	-0.34	TB
MDXVDG	X	3.061	1.270	5.44	3.127	1.054	4.47	TT
MGUPN4		1.967	0.176	0.76	2.301	0.228	0.97	TH
MYDGVF		1.731	-0.060	-0.26	2.057	-0.016	-0.07	TO
N3RAQE		1.663	-0.128	-0.55	1.892	-0.181	-0.77	LH
NH338Q	X	2.550	0.759	3.25	2.980	0.907	3.84	XX
P4DMGV		1.802	0.011	0.05	2.087	0.014	0.06	TO
Q2BXZ9		2.130	0.339	1.45	2.440	0.367	1.56	TO
QTX3JK		2.190	0.399	1.71	2.542	0.469	1.99	IF
QUAHDL		1.826	0.035	0.15	2.104	0.031	0.13	LE
QVKMNP		1.777	-0.013	-0.06	2.038	-0.035	-0.15	IN
RDLP49		1.768	-0.023	-0.10	2.097	0.024	0.10	ID
T8PHX6	X	16.625	14.834	63.57	13.411	11.338	48.04	XX
T8PM98		1.780	-0.011	-0.05	1.963	-0.110	-0.47	IM
TG8BYZ		1.851	0.060	0.26	2.205	0.132	0.56	IM
UGR6LV		1.393	-0.398	-1.70	1.779	-0.294	-1.24	LA
UQHPP9		1.936	0.145	0.62	2.213	0.140	0.59	XX
VA4Y2U		1.541	-0.250	-1.07	1.792	-0.281	-1.19	LW
VT3WPV		1.510	-0.281	-1.20	1.800	-0.273	-1.16	LH
W8DWW7		1.992	0.201	0.86	2.313	0.240	1.02	IM
WLVUTU		1.567	-0.224	-0.96	1.712	-0.361	-1.53	TA
XQP2XN		1.594	-0.197	-0.84	1.866	-0.207	-0.88	LE



Paper & Paperboard Interlaboratory Testing Program
Analysis 332
Elongation to Break - Packaging Papers
TAPPI Official Test Method T494

Report #2911S,
November 2017

WebCode	Data Flag	Sample SE49			Sample SE50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
XUNH9W		1.540	-0.251	-1.07	1.797	-0.276	-1.17	LW
XX7LWU	*	1.796	0.005	0.02	2.345	0.272	1.15	TH
Y46LT2		1.830	0.039	0.17	2.074	0.001	0.01	TK
ZXY8NB		2.225	0.434	1.86	2.391	0.319	1.35	IK

Summary Statistics	Sample SE49	Sample SE50
Grand Means	1.79 Percent	2.07 Percent
Std Dev Btw Labs	0.23 Percent	0.24 Percent

Statistics based on 39 of 44 reporting participants.

Comments on Assigned Data Flags for Test #332

- T8PHX6 (X) - Extreme Data.
- MDXVDG (X) - Data for both samples are high. Possible Systematic Error.
- C7BE89 (X) - Inconsistent in testing between samples.
- 96M2TK (X) - Inconsistent in testing between samples.
- NH338Q (X) - Data for both samples are high. Possible Systematic Error. Inconsistent within the determinations of sample SE50.

Analysis Notes:

9FAQZ8 - One determination removed from the Lab Mean of Sample SE50 per Grubb's Test at 1% risk (TAPPI 1205).

Key to Instrument Codes Reported by Participants

ID	Instron 4201	IF	Instron 3340 Series
IK	Instron 4400 Series	IM	Instron 5500 Series
IN	Instron 3360 Series	LA	L & W Autoline 300
LE	L & W Tensile Tester 066	LH	L & W Alwetron TH1 (Horizontal) SE 060
LW	L & W Tensile Tester SE062	LX	L & W (model not specified)
TA	Thwing-Albert Tensile Tester	TB	Thwing-Albert EJA/1000
TH	Thwing-Albert QC-3A	TK	Thwing-Albert Model 37-4
TO	Thwing-Albert QC-1000	TR	TMI Horizontal Tensile Tester
TT	Tinius Olsen Model MHT	XX	Instrument make/model not specified by lab



Paper & Paperboard Interlaboratory Testing Program


Report #2911S,
November 2017

Analysis 332 Elongation to Break - Packaging Papers TAPPI Official Test Method T494

Grand Mean Sample SE49 = 1.7907
Percent

Grand Mean Sample SE50 = 2.0727
Percent

ANALYSIS 332

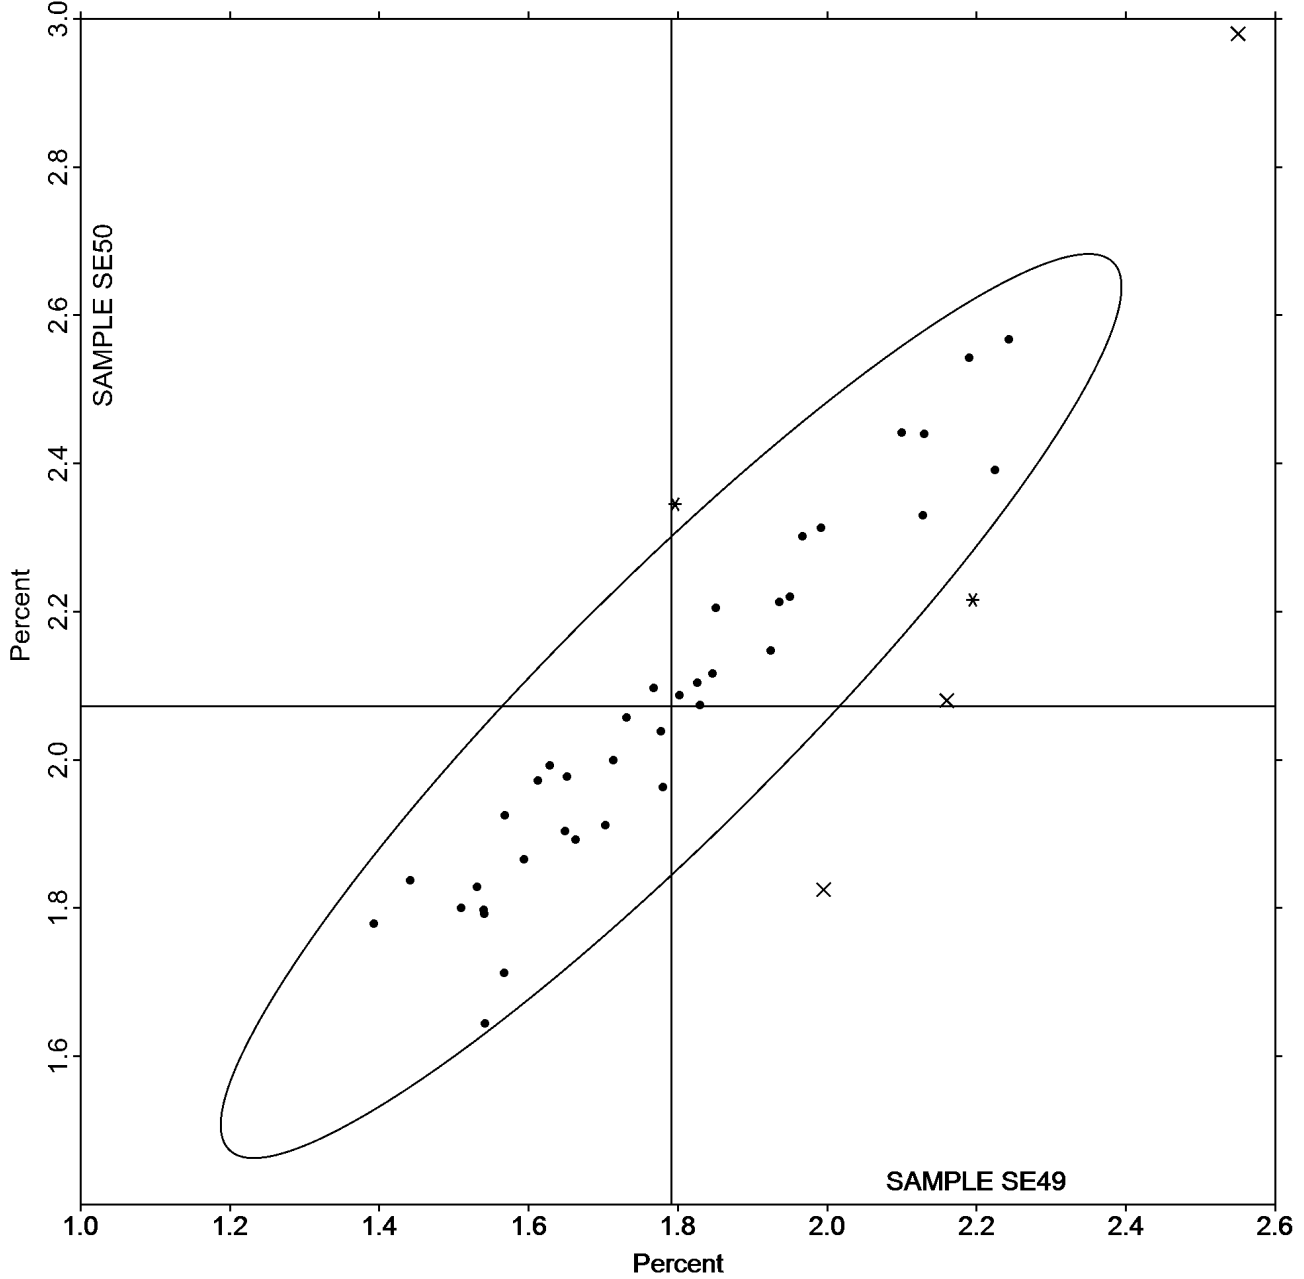



Paper & Paperboard Interlaboratory Testing Program
Analysis 334
Folding Endurance (MIT) - Double Folds
TAPPI Official Test Method T511

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SG49</u>			<u>Sample SG50</u>			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
2G7Y4H		89.30	5.42	0.30	75.20	-5.42	-0.30	MT
3X9V39		116.10	32.22	1.76	110.10	29.48	1.65	MT
778RCF		73.70	-10.18	-0.56	66.90	-13.72	-0.77	MT
EQB6LE	X	93.60	9.72	0.53	47.10	-33.52	-1.88	MT
FMAGLJ		60.60	-23.28	-1.27	61.20	-19.42	-1.09	MT
FRFET3		69.80	-14.08	-0.77	71.90	-8.72	-0.49	MT
GYUK3E		73.50	-10.38	-0.57	73.10	-7.52	-0.42	XX
Q76ULT		82.10	-1.78	-0.10	92.30	11.68	0.66	MT
QCBP6T		73.90	-9.98	-0.55	57.70	-22.92	-1.29	MT
UQHPP9		80.60	-3.28	-0.18	84.30	3.68	0.21	MT
VA4Y2U	X	61.60	-22.28	-1.22	80.40	-0.22	-0.01	MT
VZGXN6		84.50	0.62	0.03	83.60	2.98	0.17	MT
XRYBPK		118.60	34.72	1.90	110.50	29.88	1.68	MT

Summary Statistics	<u>Sample SG49</u>	<u>Sample SG50</u>
Grand Means	83.88 Double Folds	80.62 Double Folds
Stnd Dev Btwn Labs	18.27 Double Folds	17.81 Double Folds
Statistics based on 11 of 13 reporting participants.		

Comments on Assigned Data Flags for Test #334

EQB6LE (X) - Inconsistent in testing between samples.

VA4Y2U (X) - Inconsistent in testing between samples. Inconsistent within the determinations of sample SG50.

Key to Instrument Codes Reported by Participants

MT MIT - Tinius Olsen

XX Instrument make/model not specified by lab



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017

Analysis 334


Folding Endurance (MIT) - Double Folds

TAPPI Official Test Method T511

Grand Mean Sample SG49 = 83.882
Double Folds

Grand Mean Sample SG50 = 80.618
Double Folds

ANALYSIS 334

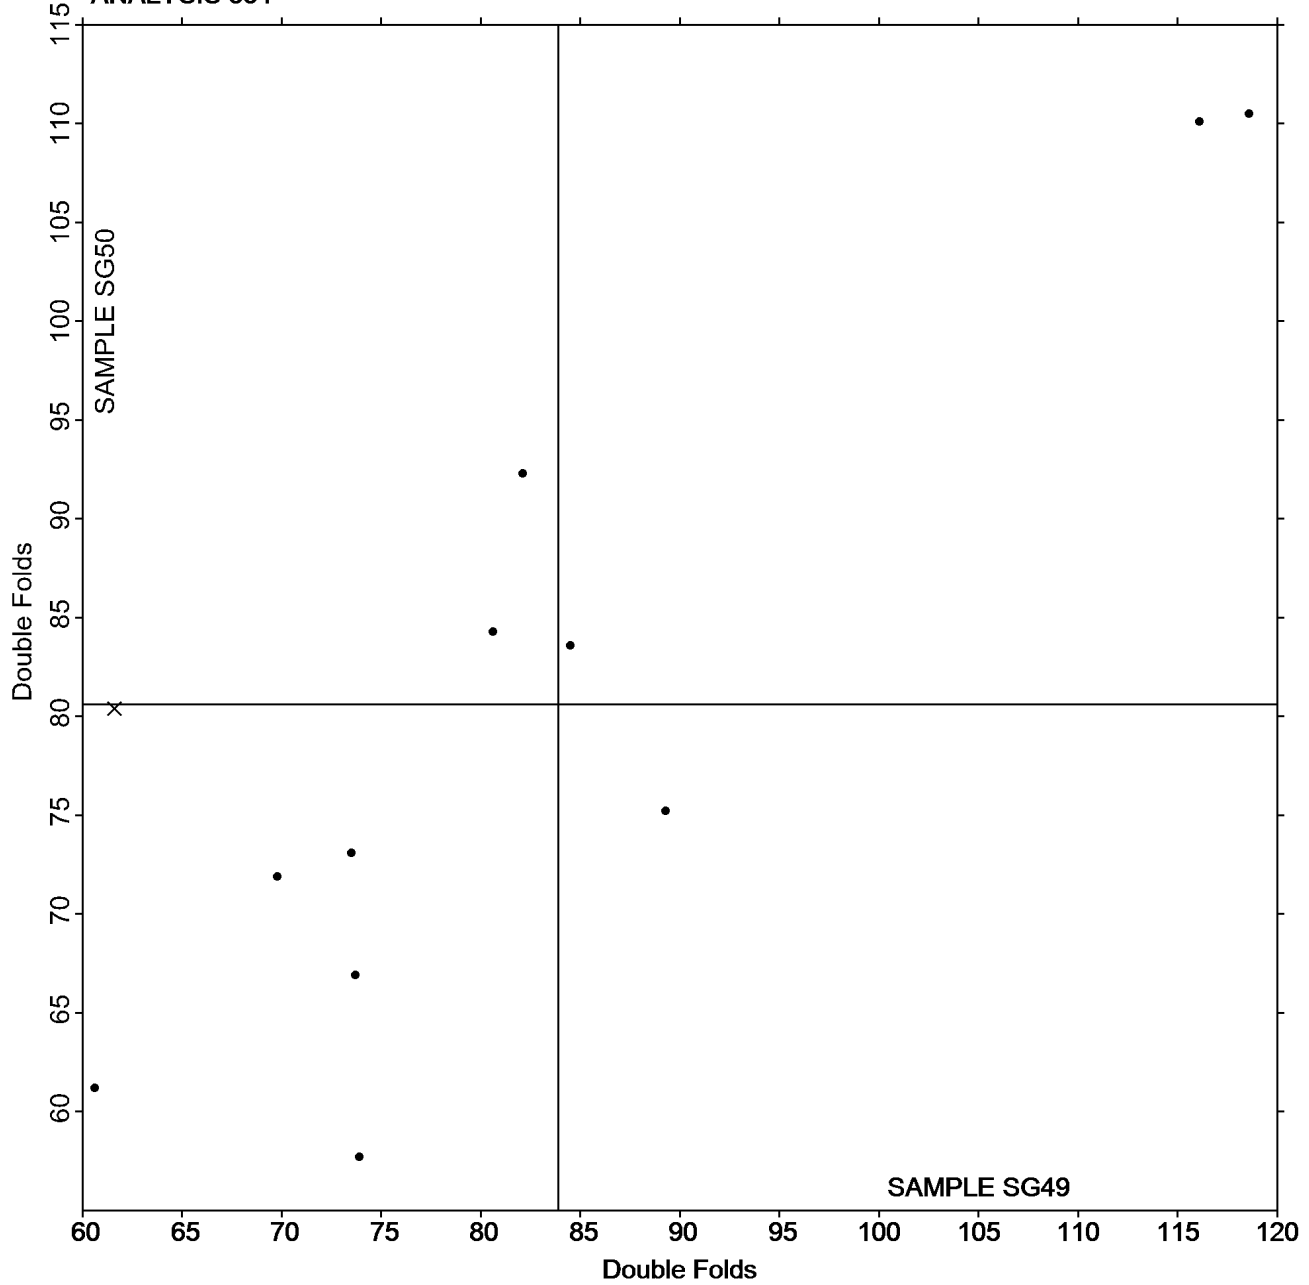

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 336
Bending Resistance, Gurley Type
TAPPI Official Test Method T543

Report #2911S,
November 2017

WebCode	Data Flag	Sample SH49			Sample SH50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
2G7Y4H		149.4	-0.9	-0.07	144.3	-0.8	-0.06
6T9NAA		161.4	11.1	0.95	148.3	3.2	0.27
7XXAUG		135.1	-15.2	-1.29	128.4	-16.6	-1.39
883W7E		149.1	-1.2	-0.10	148.3	3.2	0.27
DJB NB9		149.2	-1.1	-0.09	148.7	3.7	0.31
EQB6LE		153.8	3.5	0.30	150.2	5.2	0.43
FCMM7F		130.3	-20.0	-1.70	128.1	-17.0	-1.42
FM7YJE		153.2	2.9	0.25	146.1	1.0	0.09
GTNPJE		141.2	-9.1	-0.77	137.3	-7.7	-0.65
GYUK3E		145.4	-4.9	-0.42	144.2	-0.9	-0.07
MDXUBV	X	107.4	-42.8	-3.65	102.6	-42.5	-3.55
NBLFJF		132.5	-17.7	-1.51	123.4	-21.6	-1.81
QTX3JK		174.3	24.0	2.05	169.8	24.8	2.07
TVUHW2	X	188.4	38.1	3.25	255.2	110.1	9.21
UQHPP9		153.2	2.9	0.25	148.1	3.0	0.25
WFAULU		161.2	11.0	0.93	158.2	13.1	1.10
XLUARC		152.5	2.2	0.19	139.4	-5.6	-0.47
XRYBPK		162.7	12.4	1.06	157.9	12.8	1.07

Summary Statistics	Sample SH49	Sample SH50
Grand Means	150.28 Gurley Units	145.05 Gurley Units
Std Dev Btwn Labs	11.72 Gurley Units	11.96 Gurley Units
Statistics based on 16 of 18 reporting participants.		

Comments on Assigned Data Flags for Test #336

MDXUBV (X) - Data for both samples are low. Possible Systematic Error.


TVUHW2 (X) - Extreme Data.



Analysis 336
Bending Resistance, Gurley Type
TAPPI Official Test Method T543

Grand Mean Sample SH49 = 150.28
Gurley Units

Grand Mean Sample SH50 = 145.05
Gurley Units

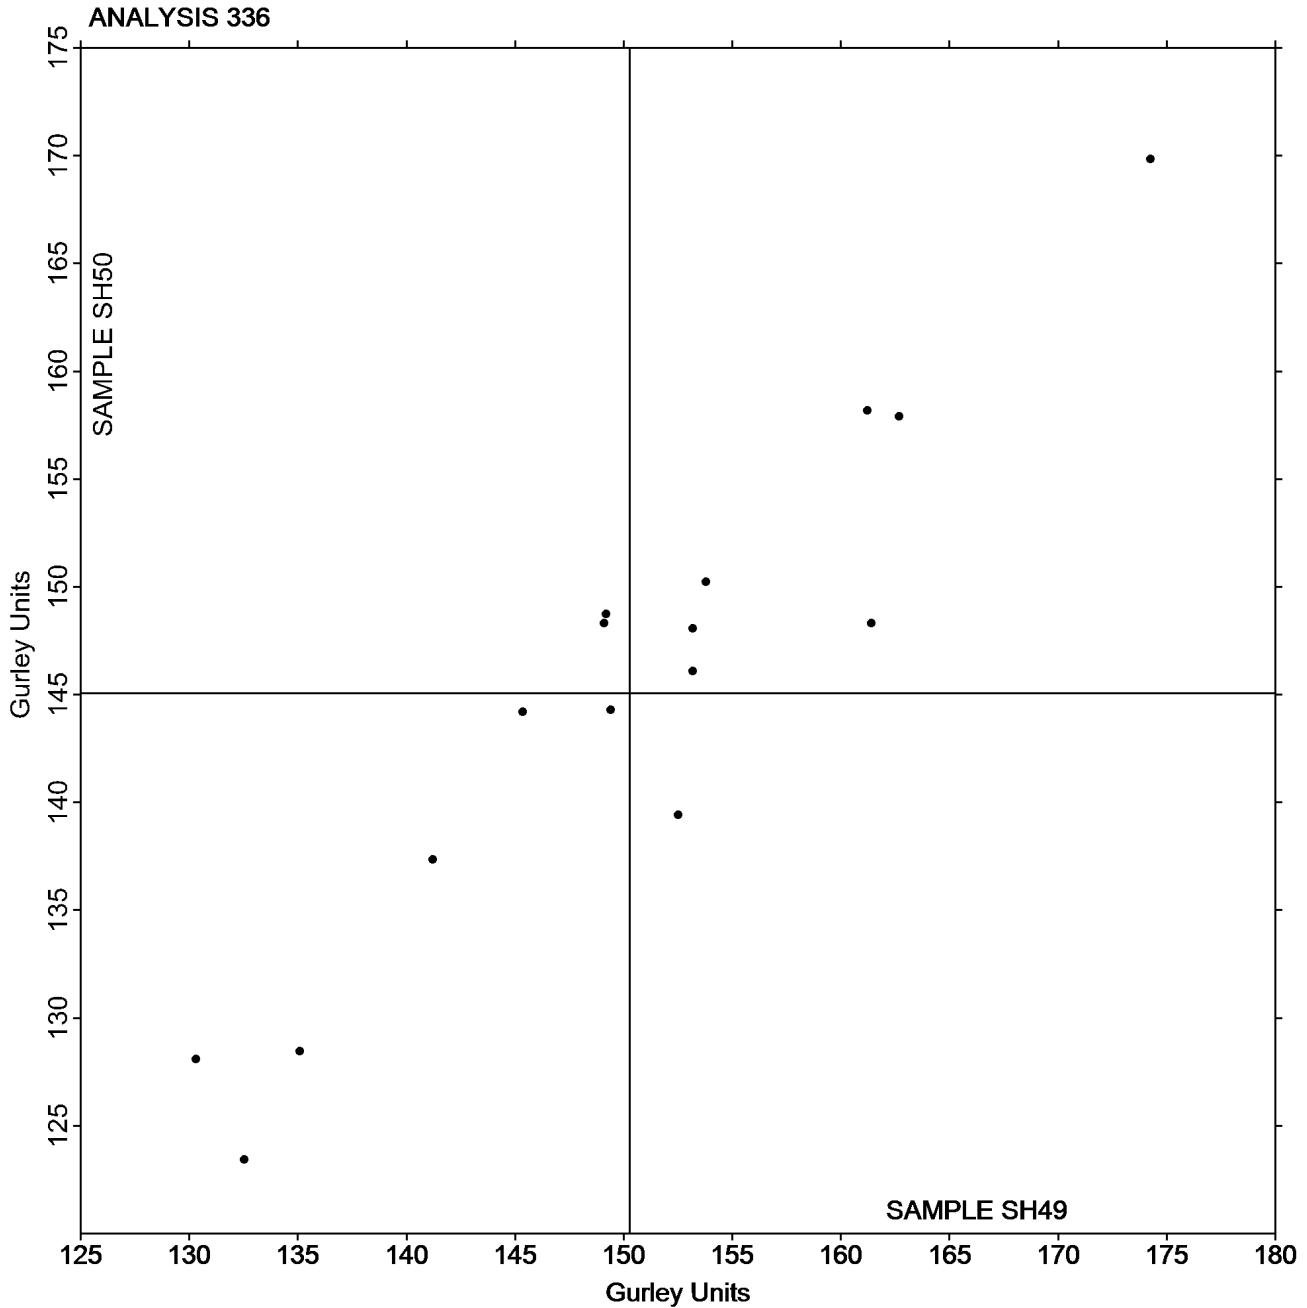

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 338
Bending Resistance, Taber Type - 0 to 10 Units
TAPPI Official Test Method T566

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SJ49</u>			<u>Sample SJ50</u>		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
2G7Y4H		2.209	0.018	0.09	2.004	-0.127	-0.68
4AFC2N		2.263	0.072	0.36	2.221	0.090	0.49
778RCF		2.406	0.215	1.07	2.373	0.242	1.30
AHRGEG		2.299	0.108	0.54	2.138	0.007	0.04
DJB NB9		2.473	0.282	1.40	2.423	0.292	1.57
DJDDGR		1.792	-0.399	-1.99	1.811	-0.320	-1.72
FM7YJE		2.070	-0.121	-0.60	2.089	-0.042	-0.23
QCBP6T		2.303	0.112	0.56	2.090	-0.041	-0.22
QTX3JK		2.262	0.071	0.35	2.238	0.107	0.58
QVKMNP	X	3.780	1.589	7.91	3.910	1.779	9.59
U46RAL	X	1.046	-1.145	-5.70	1.019	-1.112	-5.99
XUNH9W		1.960	-0.231	-1.15	1.890	-0.241	-1.30
ZMEABR		2.066	-0.125	-0.62	2.163	0.032	0.17

Summary Statistics	<u>Sample SJ49</u>	<u>Sample SJ50</u>
Grand Means	2.19 Taber Units	2.13 Taber Units
Std Dev Btwn Labs	0.20 Taber Units	0.19 Taber Units
Statistics based on 11 of 13 reporting participants.		

Comments on Assigned Data Flags for Test #338

QVKMNP (X) - Extreme Data.

U46RAL (X) - Data for both samples are low. Possible Systematic Error.

Analysis Notes:

ZMEABR - One determination removed from the Lab Mean of Sample SJ49 per Grubb's Test at 1% risk (TAPPI 1205).



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017


Analysis 338

Bending Resistance, Taber Type - 0 to 10 Units

TAPPI Official Test Method T566

Grand Mean Sample SJ49 = 2.1910
Taber Units

Grand Mean Sample SJ50 = 2.1308
Taber Units

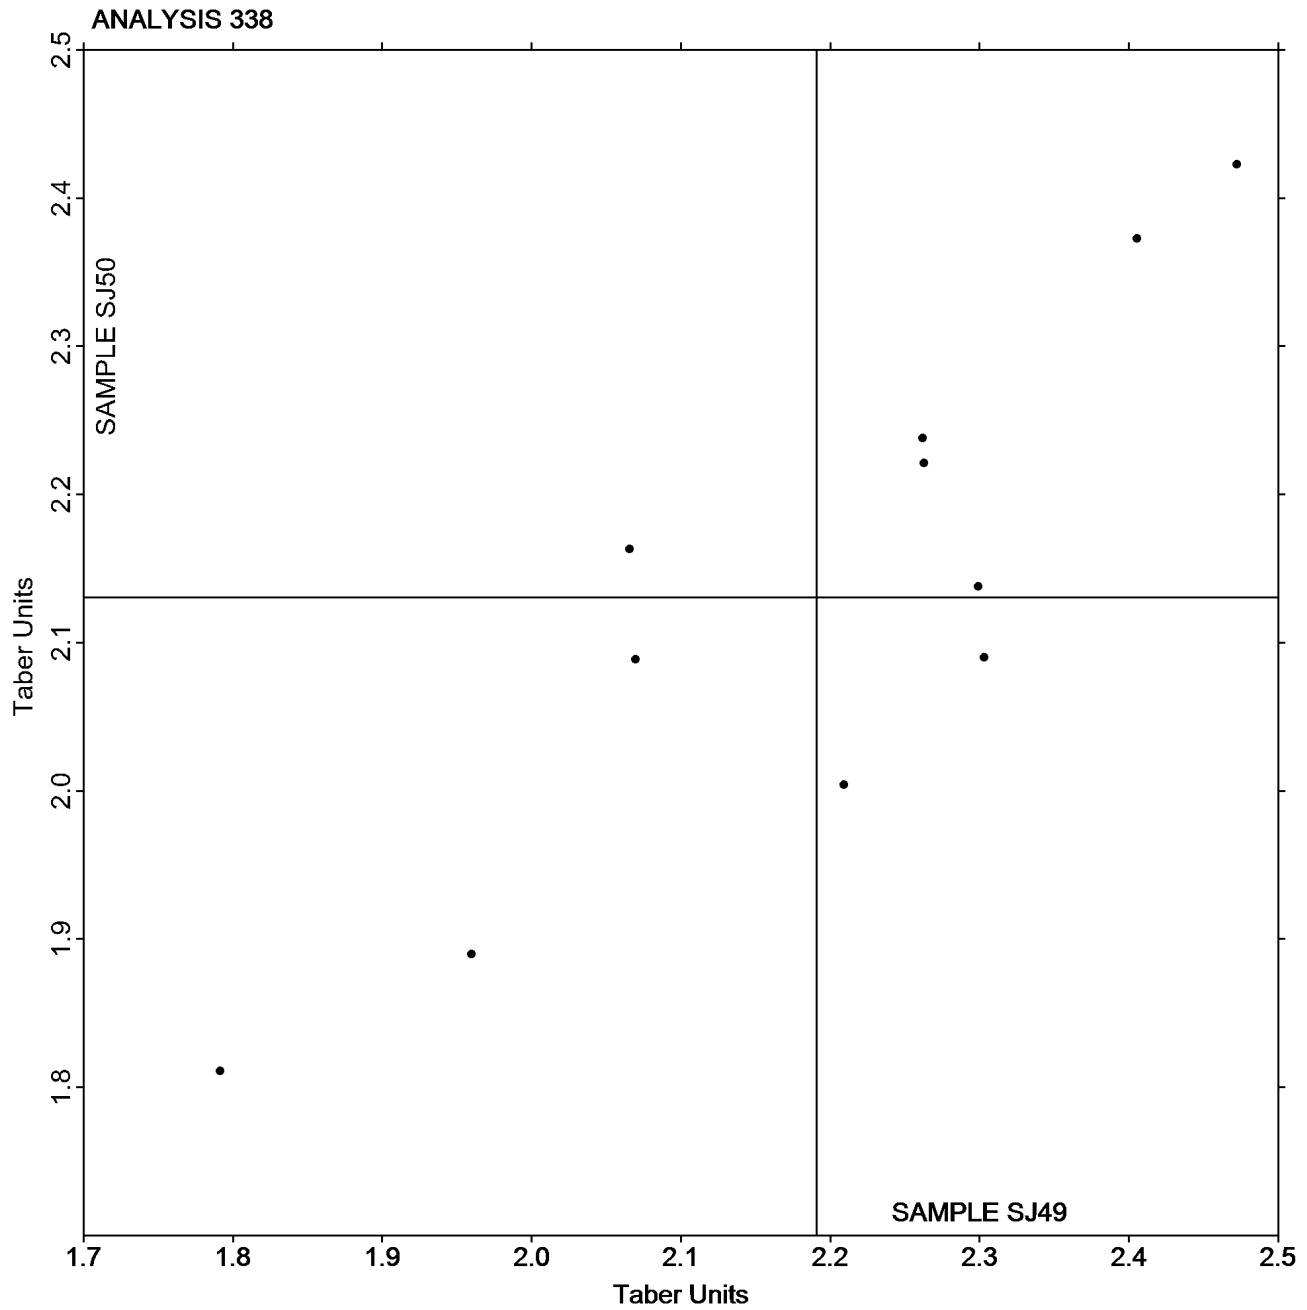

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 339
Bending Resistance, Taber Type - 10 to 100 Taber Units
TAPPI Official Test Method T489

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SQ49</u>			<u>Sample SQ50</u>		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
2G7Y4H		111.9	0.9	0.11	110.8	-1.2	-0.16
62XC6C		105.9	-5.1	-0.65	105.6	-6.3	-0.86
6T9NAA		108.5	-2.5	-0.32	108.7	-3.3	-0.45
8NK38C		108.1	-2.9	-0.37	110.8	-1.2	-0.17
GZP2GW	X	19.1	-91.9	-11.77	19.5	-92.5	-12.56
LP8D86		99.7	-11.3	-1.44	107.8	-4.2	-0.57
UCX8W6	X	31.5	-79.5	-10.19	36.8	-75.2	-10.21
UGR6LV		101.2	-9.8	-1.25	103.1	-8.9	-1.21
VA4Y2U		120.4	9.4	1.20	120.3	8.3	1.13
WFNFVV		114.3	3.3	0.42	128.0	16.0	2.18
XLUARC		116.5	5.5	0.70	114.8	2.8	0.38
XUNH9W		123.5	12.5	1.60	110.0	-2.0	-0.27

Summary Statistics	<u>Sample SQ49</u>	<u>Sample SQ50</u>
Grand Means	110.99 Taber Units	111.98 Taber Units
Std Dev Btwn Labs	7.81 Taber Units	7.36 Taber Units
Statistics based on 10 of 12 reporting participants.		

Comments on Assigned Data Flags for Test #339

UCX8W6 (X) - Extreme Data.

GZP2GW (X) - Extreme Data.



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017


Analysis 339

Bending Resistance, Taber Type - 10 to 100 Taber Units

TAPPI Official Test Method T489

Grand Mean Sample SQ49 = 110.99
Taber Units

Grand Mean Sample SQ50 = 111.98
Taber Units

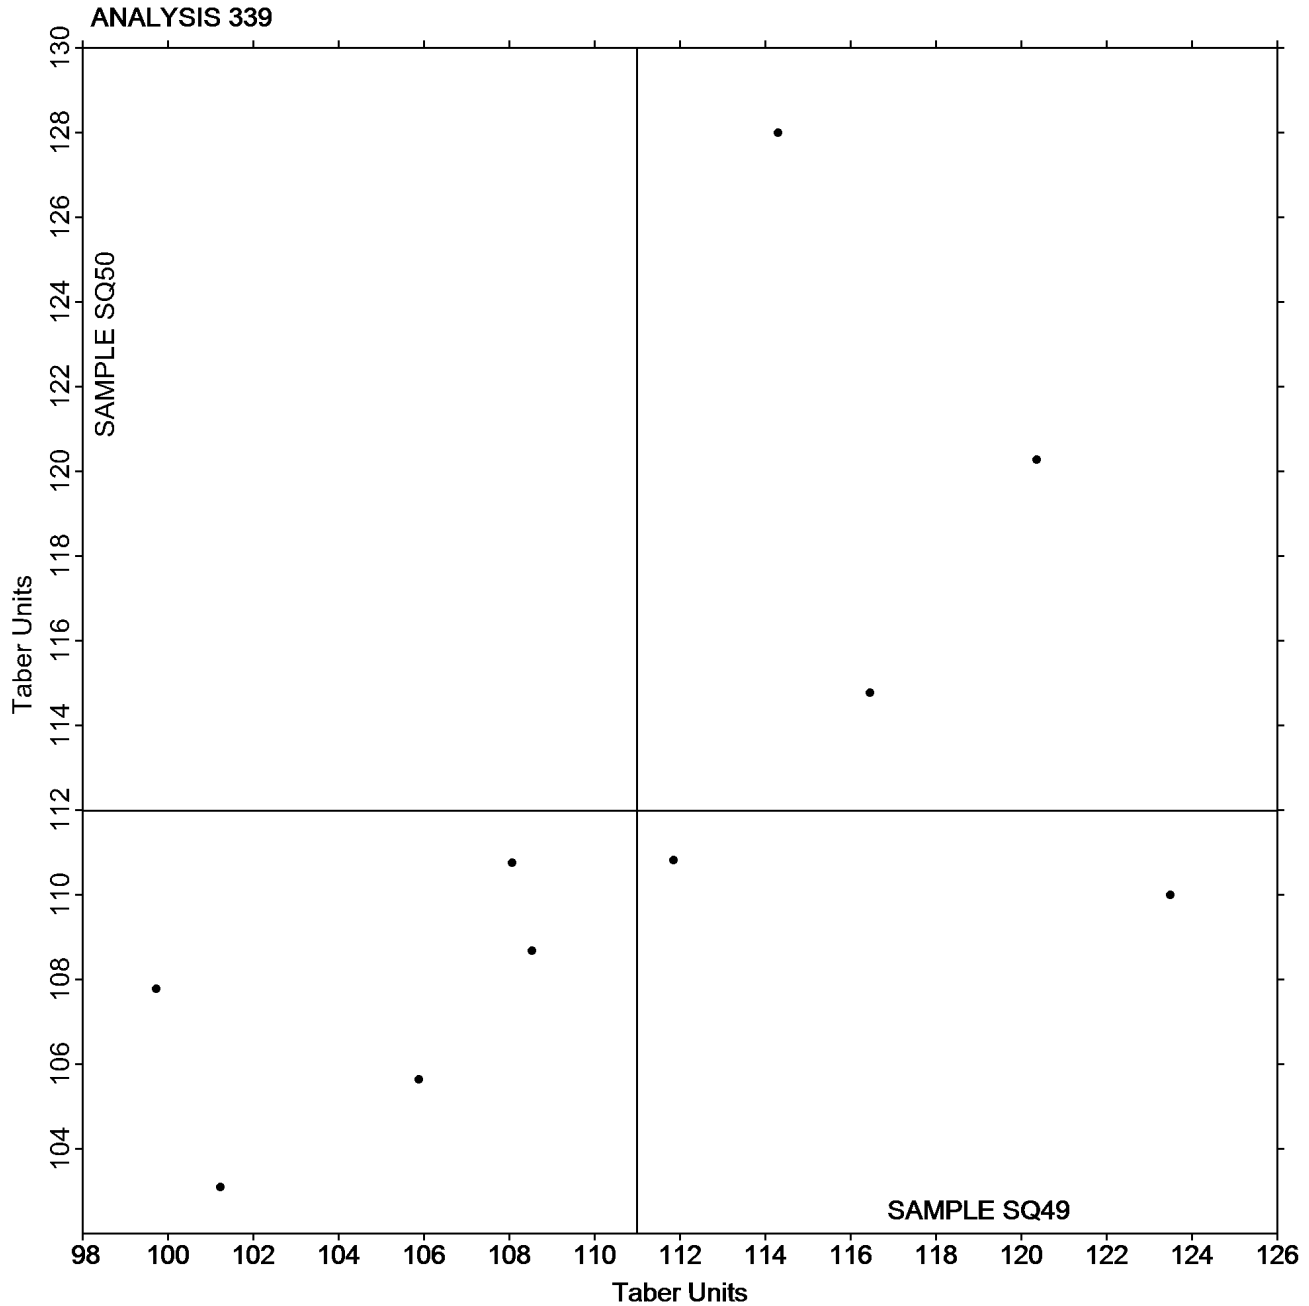

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program

**Report #2911S,
November 2017**

Analysis 340

Bending Resistance, Taber Type - 50 to 500 Taber Units - Recycled Paperboard

TAPPI Official Test Method T489

WebCode	Data Flag	Sample ST49			Sample ST50		
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV
4YHM79		281.7	-0.2	-0.02	290.3	2.2	0.18
87RUHU		278.1	-3.8	-0.39	271.4	-16.8	-1.42
C6YQT4		283.7	1.8	0.19	288.0	-0.1	-0.01
DD8GXR		265.3	-16.6	-1.74	274.2	-14.0	-1.18
FMAGLJ		273.0	-8.9	-0.93	277.8	-10.3	-0.87
GAWZRJ		289.0	7.1	0.75	293.2	5.1	0.43
JHL7YP	X	249.2	-32.7	-3.42	268.5	-19.6	-1.66
LYHD6M		282.1	0.2	0.03	291.9	3.8	0.32
QHUZ9W		287.7	5.8	0.61	288.5	0.4	0.03
QJ8K6C		269.6	-12.2	-1.28	279.7	-8.4	-0.71
UQHPP9		281.6	-0.2	-0.03	282.4	-5.8	-0.49
VA4Y2U		295.1	13.3	1.39	311.9	23.7	2.01
WWE9XG		274.1	-7.8	-0.81	284.0	-4.1	-0.35
XLUARC		284.4	2.5	0.26	290.6	2.5	0.21
XUNH9W		280.0	-1.9	-0.19	285.0	-3.1	-0.27
Y4A4V7		302.4	20.5	2.15	313.3	25.2	2.12

Summary Statistics	Sample ST49	Sample ST50
Grand Means	281.85 Taber Units	288.14 Taber Units
Std Dev Btwn Labs	9.54 Taber Units	11.84 Taber Units
Statistics based on 15 of 16 reporting participants.		

Comments on Assigned Data Flags for Test #340

JHL7YP (X) - Data for sample ST49 are low.

Analysis Notes:

4YHM79 - Data appear to be reported as g-cm , not mN-m as indicated on datasheet. Units corrected by CTS.

QJ8K6C - Data appear to be reported as mN-m, not g-cm as indicated on datasheet. Units corrected by CTS.



Paper & Paperboard Interlaboratory Testing Program

Report #2911S,
November 2017


Analysis 340

Bending Resistance, Taber Type - 50 to 500 Taber Units - Recycled Paperboard

TAPPI Official Test Method T489

Grand Mean Sample ST49 = 281.85
Taber Units

Grand Mean Sample ST50 = 288.14
Taber Units

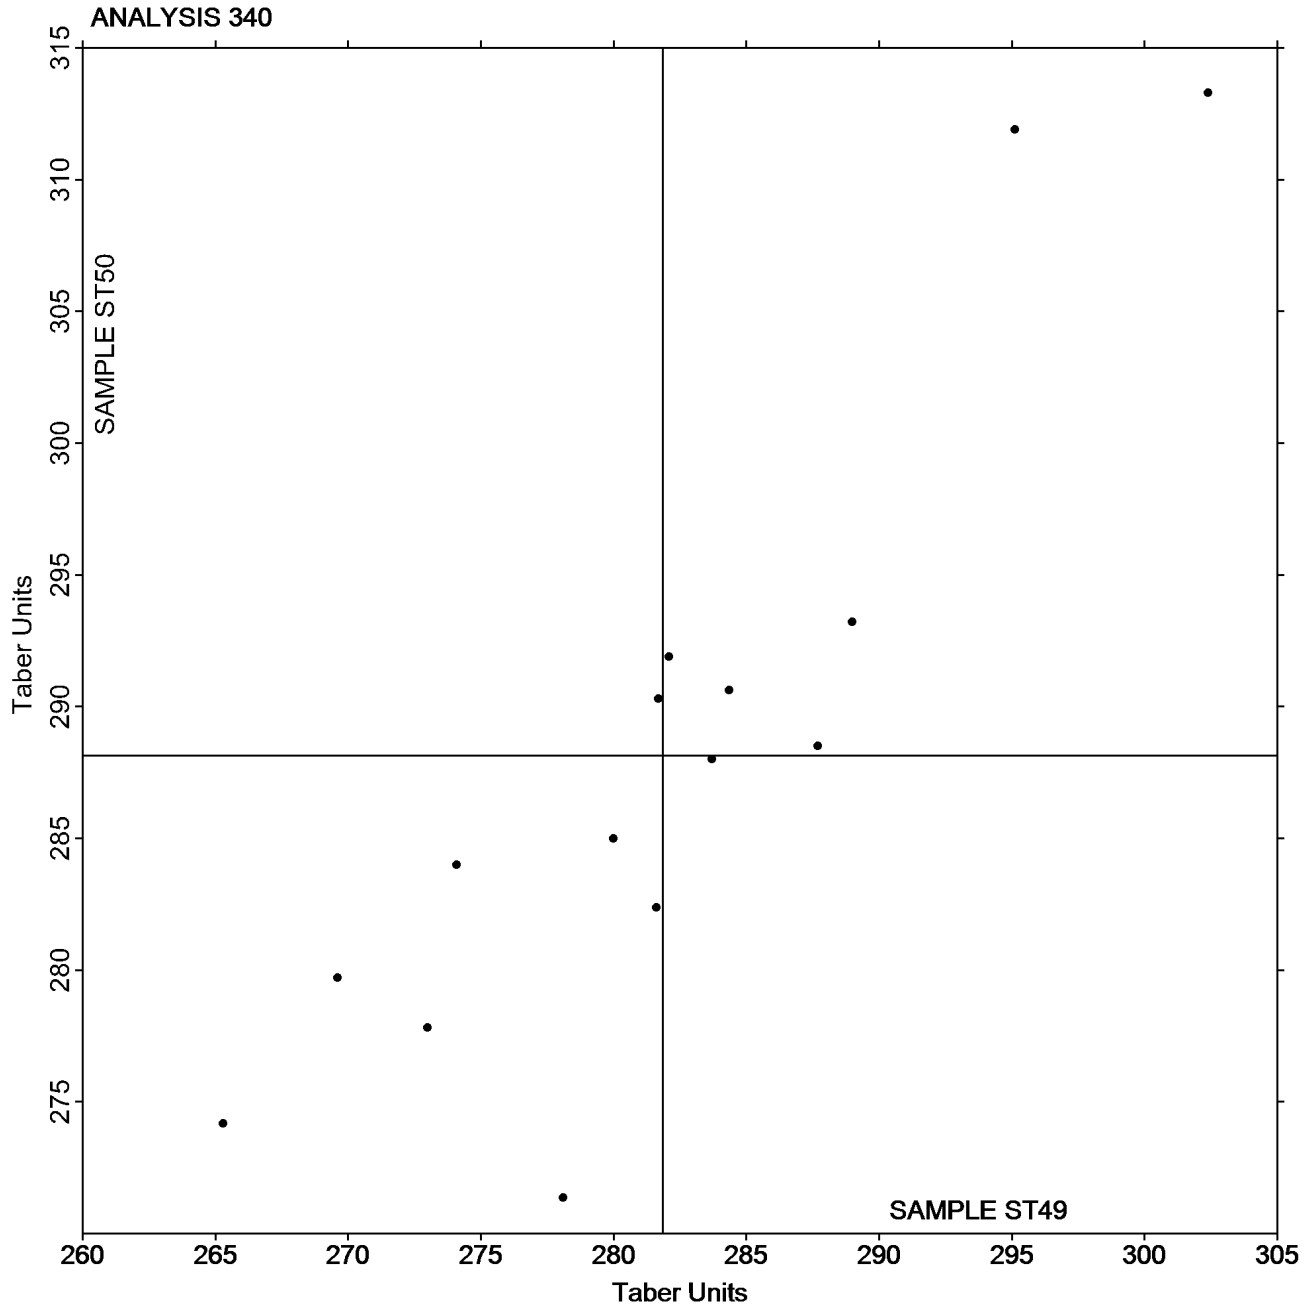

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 343
Z-Direction Tensile
TAPPI Official Test Method T541

Report #2911S,
November 2017

WebCode	Data Flag	Sample SM49			Sample SM50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
4FPJP9		71.00	5.67	0.85	69.60	3.61	0.60	TA
778RCF		63.66	-1.67	-0.25	60.76	-5.23	-0.87	CD
87RUHU		72.20	6.87	1.04	74.00	8.01	1.33	CA
8NK38C		78.36	13.03	1.96	75.32	9.33	1.55	TA
8PJY32		64.64	-0.69	-0.10	64.60	-1.39	-0.23	DT
9JNN79		63.40	-1.93	-0.29	61.60	-4.39	-0.73	XX
CT3K2Q		58.40	-6.94	-1.05	58.38	-7.61	-1.26	LW
DJDDGR		72.76	7.43	1.12	76.84	10.85	1.80	DT
FMAGLJ		58.06	-7.27	-1.10	62.94	-3.05	-0.51	LW
GZP2GW		61.33	-4.01	-0.60	66.85	0.86	0.14	LW
LP8D86		59.54	-5.79	-0.87	59.25	-6.74	-1.12	TZ
Q2BXZ9		58.40	-6.93	-1.05	58.80	-7.19	-1.19	TA
QJ8K6C		57.73	-7.61	-1.15	59.26	-6.73	-1.11	LX
QTX3JK		61.14	-4.19	-0.63	66.30	0.31	0.05	TL
QUAHDL		65.84	0.51	0.08	67.60	1.61	0.27	TA
VA4Y2U		75.74	10.41	1.57	71.98	5.99	0.99	LW
XECYDB		68.48	3.15	0.47	67.76	1.77	0.29	DT

Summary Statistics	Sample SM49	Sample SM50
Grand Means	65.33 psi	65.99 psi
Std Dev Btwn Labs	6.63 psi	6.03 psi
Statistics based on 17 of 17 reporting participants.		

Key to Instrument Codes Reported by Participants

CA	CSI CS-163	CD	CSI CS-163D
DT	Dek-Tron DCS-163A ZDT Tester	LW	L & W ZD Tensile Tester
LX	L & W (model not specified)	TA	Thwing-Albert Tensile Tester
TL	TMI Lab Master	TZ	TMI Monitor/ZDT Tester
XX	Instrument make/model not specified by lab		




Paper & Paperboard Interlaboratory Testing Program
Analysis 343
Z-Direction Tensile
TAPPI Official Test Method T541

Report #2911S,
November 2017

Grand Mean Sample SM49 = 65.334
psi

Grand Mean Sample SM50 = 65.991
psi

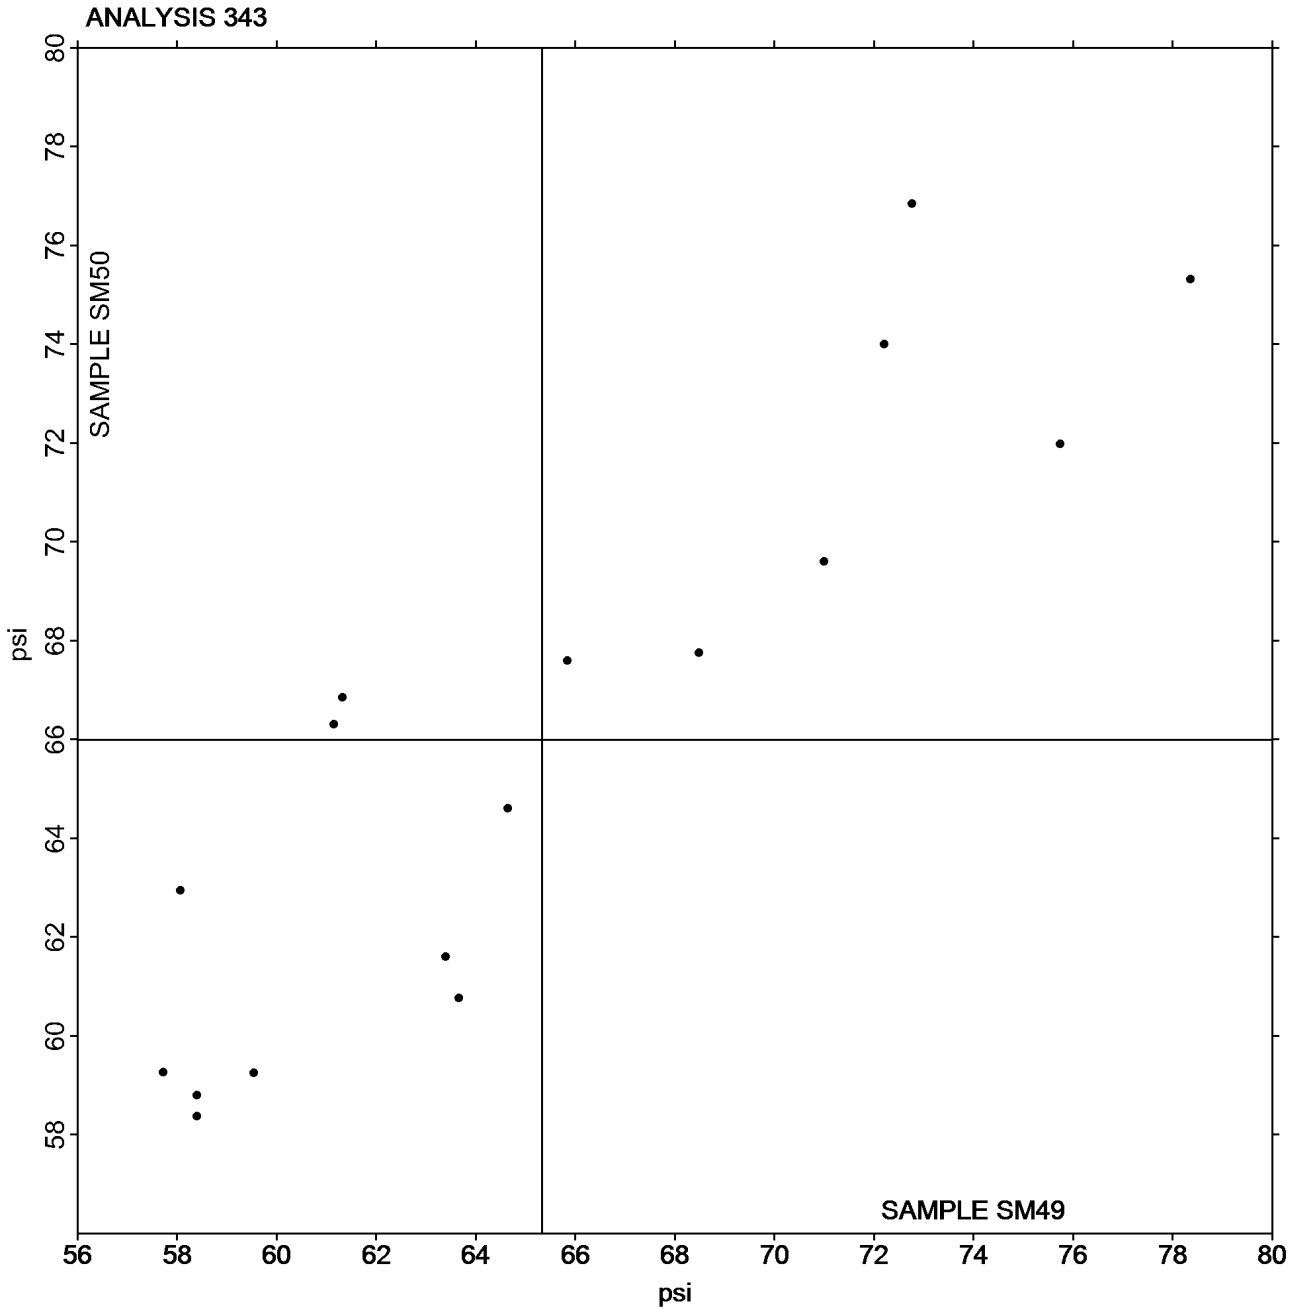

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 345
Z-Direction Tensile, Recycled Paperboard
TAPPI Official Test Method T541

Report #2911S,
November 2017

WebCode	Data Flag	Sample SZ49			Sample SZ50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
2ABYRB		35.20	0.06	0.02	35.12	-0.20	-0.08	CD
4YHM79		35.68	0.54	0.18	34.76	-0.56	-0.22	CD
6MK47U		38.24	3.10	1.04	37.48	2.17	0.86	CH
882X9Y		36.12	0.97	0.33	36.16	0.85	0.33	TA
9PYKAH		33.38	-1.76	-0.59	34.52	-0.80	-0.32	DP
AZDYQP		31.52	-3.62	-1.22	33.86	-1.46	-0.58	LW
C6YQT4		34.56	-0.58	-0.20	35.18	-0.14	-0.05	TL
DD8GXR		32.80	-2.34	-0.79	34.80	-0.52	-0.20	TA
JHL7YP		36.00	0.86	0.29	34.00	-1.32	-0.52	CA
LYHD6M		36.80	1.66	0.56	36.40	1.08	0.43	CA
QHUZ9W		39.76	4.62	1.55	39.86	4.54	1.80	TA
UQHPP9		33.60	-1.54	-0.52	32.60	-2.72	-1.07	CA
WWE9XG		33.56	-1.58	-0.53	34.98	-0.34	-0.13	TZ
XLUARC		30.02	-5.12	-1.72	30.84	-4.48	-1.77	CA
Y63WN4		33.52	-1.62	-0.55	33.48	-1.84	-0.73	LW
ZXY8NB		41.55	6.41	2.15	41.03	5.72	2.26	PG

Summary Statistics	Sample SZ49	Sample SZ50
Grand Means	35.14 psi	35.32 psi
Std Dev Btwn Labs	2.97 psi	2.53 psi
Statistics based on 16 of 16 reporting participants.		

Key to Instrument Codes Reported by Participants

CA	CSI CS-163	CD	CSI CS-163D
CH	Chatillon Ametek	DP	Dek-Tron XP Series
LW	L & W ZD Tensile Tester	PG	Perkins Model A Mullen Tester
TA	Thwing-Albert Tensile Tester	TL	TMI Lab Master
TZ	TMI Monitor/ZDT Tester		




Paper & Paperboard Interlaboratory Testing Program
Analysis 345
Z-Direction Tensile, Recycled Paperboard
TAPPI Official Test Method T541

Report #2911S,
November 2017

Grand Mean Sample SZ49 = 35.144
psi

Grand Mean Sample SZ50 = 35.317
psi

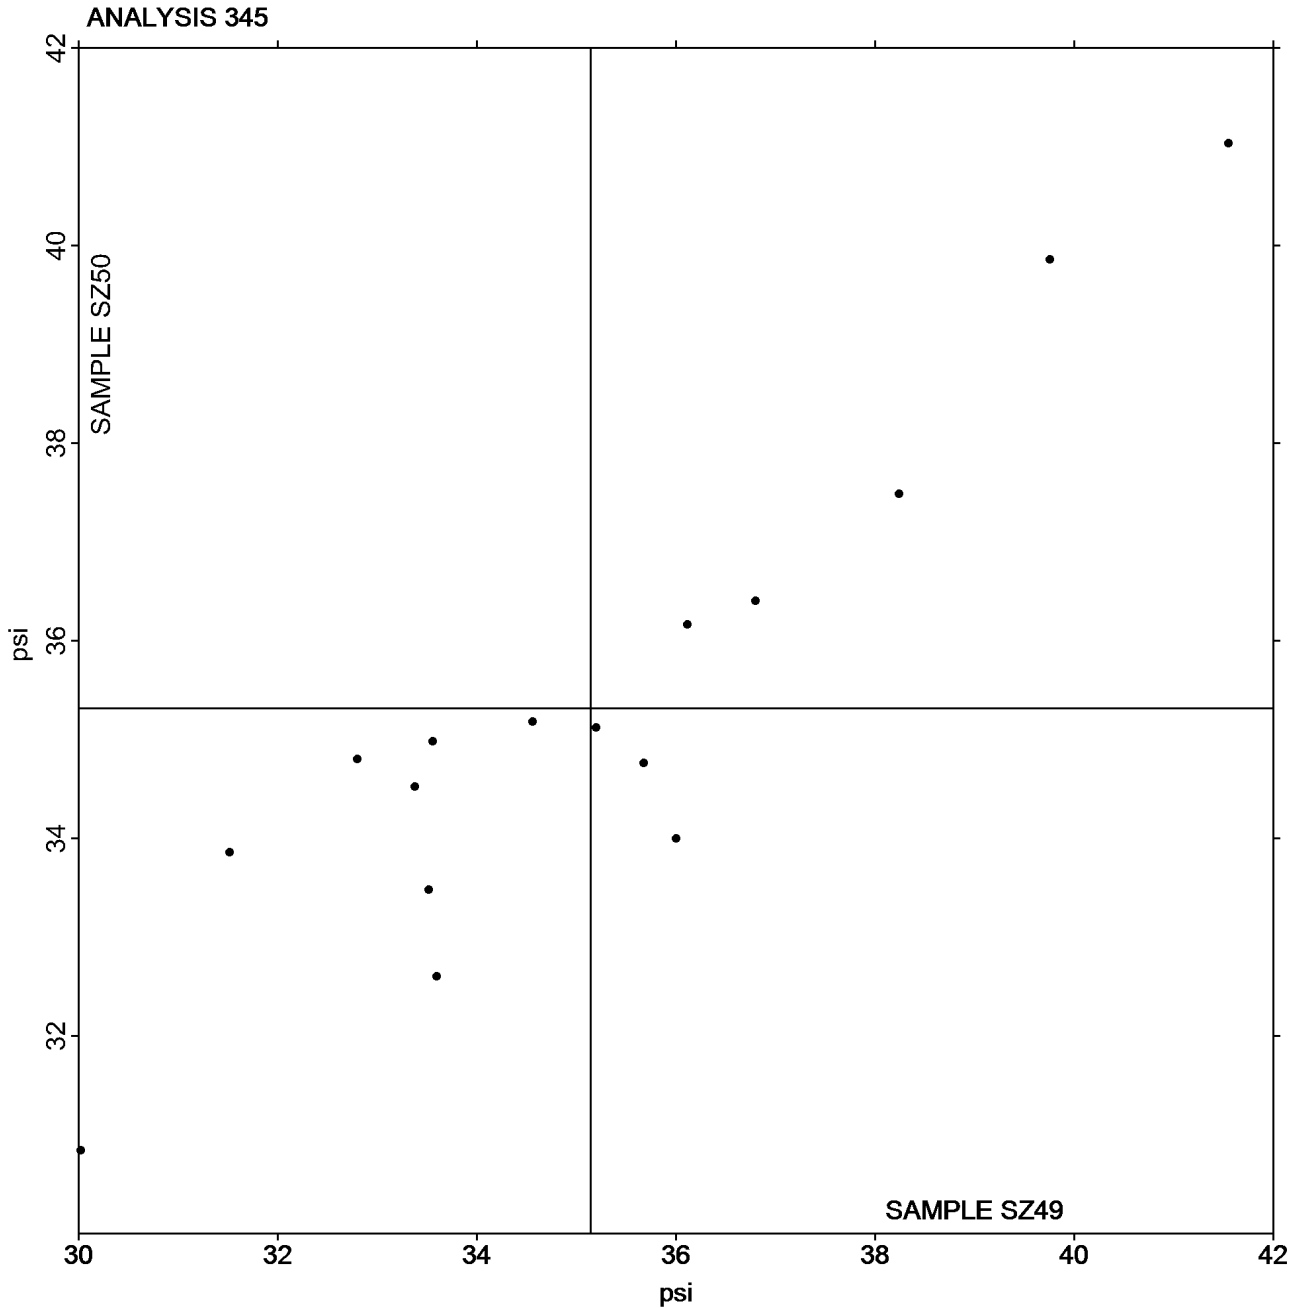

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 348
Internal Bond Strength - Modified Scott Mechanics
TAPPI Provisional Test Method T569

Report #2911S,
November 2017

WebCode	Data Flag	Sample SN49			Sample SN50			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
2G7Y4H		177.4	13.7	1.48	168.4	5.9	0.62	HY
4FPJP9		179.6	15.9	1.71	177.6	15.1	1.59	HY
778RCF		179.0	15.4	1.65	180.2	17.8	1.87	HY
7TPYPU		162.3	-1.4	-0.15	156.0	-6.5	-0.68	HY
7XXAUG		152.4	-11.3	-1.21	158.4	-4.1	-0.43	HY
8NK38C		169.6	5.9	0.64	172.0	9.5	1.00	HZ
B7VM6R		157.0	-6.7	-0.72	156.2	-6.3	-0.66	HZ
DD8GXR		163.4	-0.3	-0.03	159.0	-3.5	-0.36	HY
DJB NB9		155.6	-8.0	-0.87	154.5	-8.0	-0.84	KR
FMAGLJ		166.0	2.3	0.25	165.8	3.3	0.35	HZ
LP8D86		159.2	-4.5	-0.48	151.6	-10.9	-1.14	HY
MDXUBV		157.3	-6.4	-0.68	163.3	0.8	0.09	HY
MYDGVF		162.6	-1.1	-0.12	162.6	0.1	0.02	HY
NBLFJF		160.8	-2.9	-0.31	158.2	-4.3	-0.45	HY
QUAHDL		172.4	8.7	0.94	178.4	15.9	1.67	HY
UQHPP9		164.4	0.7	0.08	151.2	-11.3	-1.18	HZ
VA4Y2U		162.6	-1.1	-0.12	161.2	-1.3	-0.13	HY
XRYBPK		144.6	-19.1	-2.05	149.6	-12.9	-1.35	HY

Summary Statistics	Sample SN49	Sample SN50
Grand Means	163.68 1000th ft-lbs	162.45 1000th ft-lbs
Std Dev Btwn Labs	9.29 1000th ft-lbs	9.52 1000th ft-lbs
Statistics based on 18 of 18 reporting participants.		

Key to Instrument Codes Reported by Participants

HY Huygen Digitized Scott Internal Bond Tester HZ Huygen Internal Bond Tester with AccuPress
KR Kumagai Riki Kogyo Internal Bond Tester




Paper & Paperboard Interlaboratory Testing Program
Analysis 348
Internal Bond Strength - Modified Scott Mechanics
TAPPI Provisional Test Method T569

Report #2911S,
November 2017

Grand Mean Sample SN49 = 163.68
1000th ft-lbs

Grand Mean Sample SN50 = 162.45
1000th ft-lbs

ANALYSIS 348

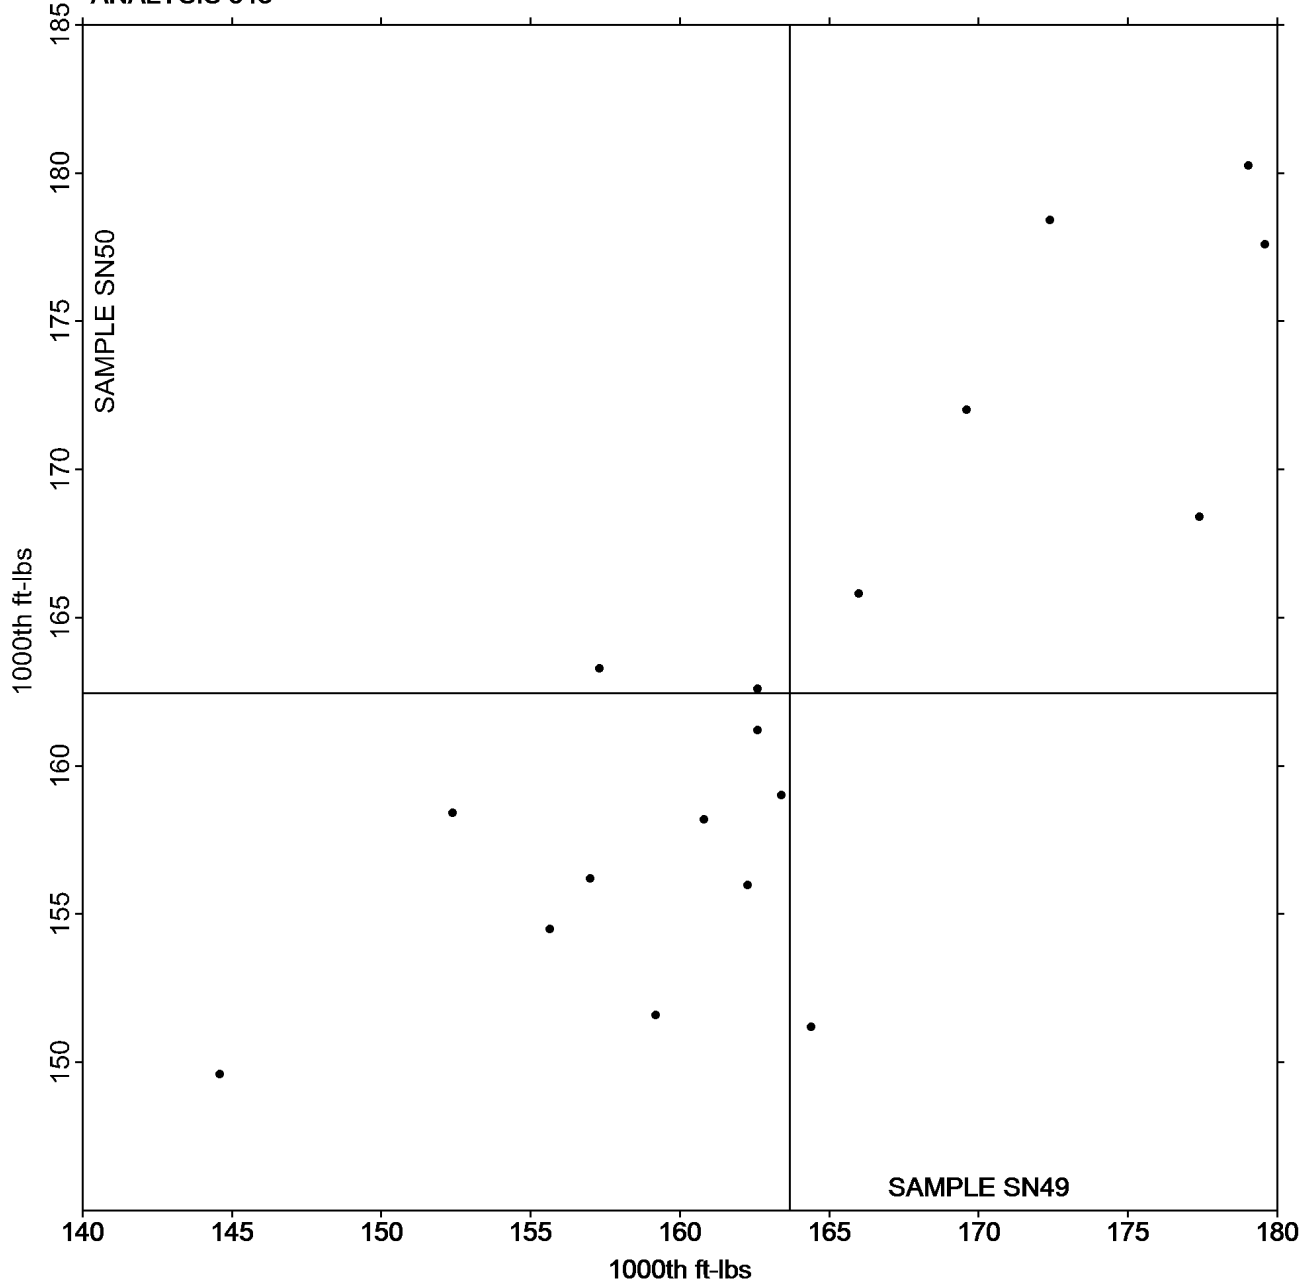

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.



Paper & Paperboard Interlaboratory Testing Program
Analysis 349
Internal Bond Strength - Scott Bond Models
TAPPI Provisional Test Method T569

Report #2911S,
November 2017

WebCode	Data Flag	<u>Sample SP49</u>			<u>Sample SP50</u>			Instr Code
		Lab Mean	Diff from Grand Mean	CPV	Lab Mean	Diff from Grand Mean	CPV	
6MK47U		145.2	-6.6	-0.28	164.4	13.6	0.63	TM
77RQ8R		151.6	-0.2	-0.01	163.6	12.8	0.59	SC
92UQ72		128.6	-23.2	-0.97	126.4	-24.4	-1.13	TM
JRMTN2		146.0	-5.8	-0.24	132.7	-18.1	-0.84	XX
N3RAQE		140.4	-11.4	-0.48	138.6	-12.2	-0.57	TM
NH338Q		198.0	46.2	1.94	179.0	28.2	1.31	XX
QJ8K6C		106.2	-45.6	-1.91	108.7	-42.1	-1.95	TM
X93RPR		161.2	9.4	0.39	161.0	10.2	0.47	SC
XUNH9W		173.4	21.6	0.91	172.0	21.2	0.98	XX
Y63WN4		137.2	-14.6	-0.61	135.8	-15.0	-0.70	XX
Z9TUAD		172.3	20.5	0.86	167.0	16.2	0.75	XX
ZXY8NB		161.4	9.6	0.40	160.6	9.8	0.45	TM

Summary Statistics	<u>Sample SP49</u>	<u>Sample SP50</u>
Grand Means	151.80 1000th ft-lbs	150.81 1000th ft-lbs
Stnd Dev Btwn Labs	23.82 1000th ft-lbs	21.59 1000th ft-lbs
Statistics based on 12 of 12 reporting participants.		

Key to Instrument Codes Reported by Participants

- SC Scott Internal Bond Tester (Manual) TM TMI Monitor/Internal Bond Tester
 XX Instrument make/model not specified by lab




Paper & Paperboard Interlaboratory Testing Program
Analysis 349
Internal Bond Strength - Scott Bond Models
TAPPI Provisional Test Method T569

Report #2911S,
November 2017

Grand Mean Sample SP49 = 151.80
1000th ft-lbs

Grand Mean Sample SP50 = 150.81
1000th ft-lbs

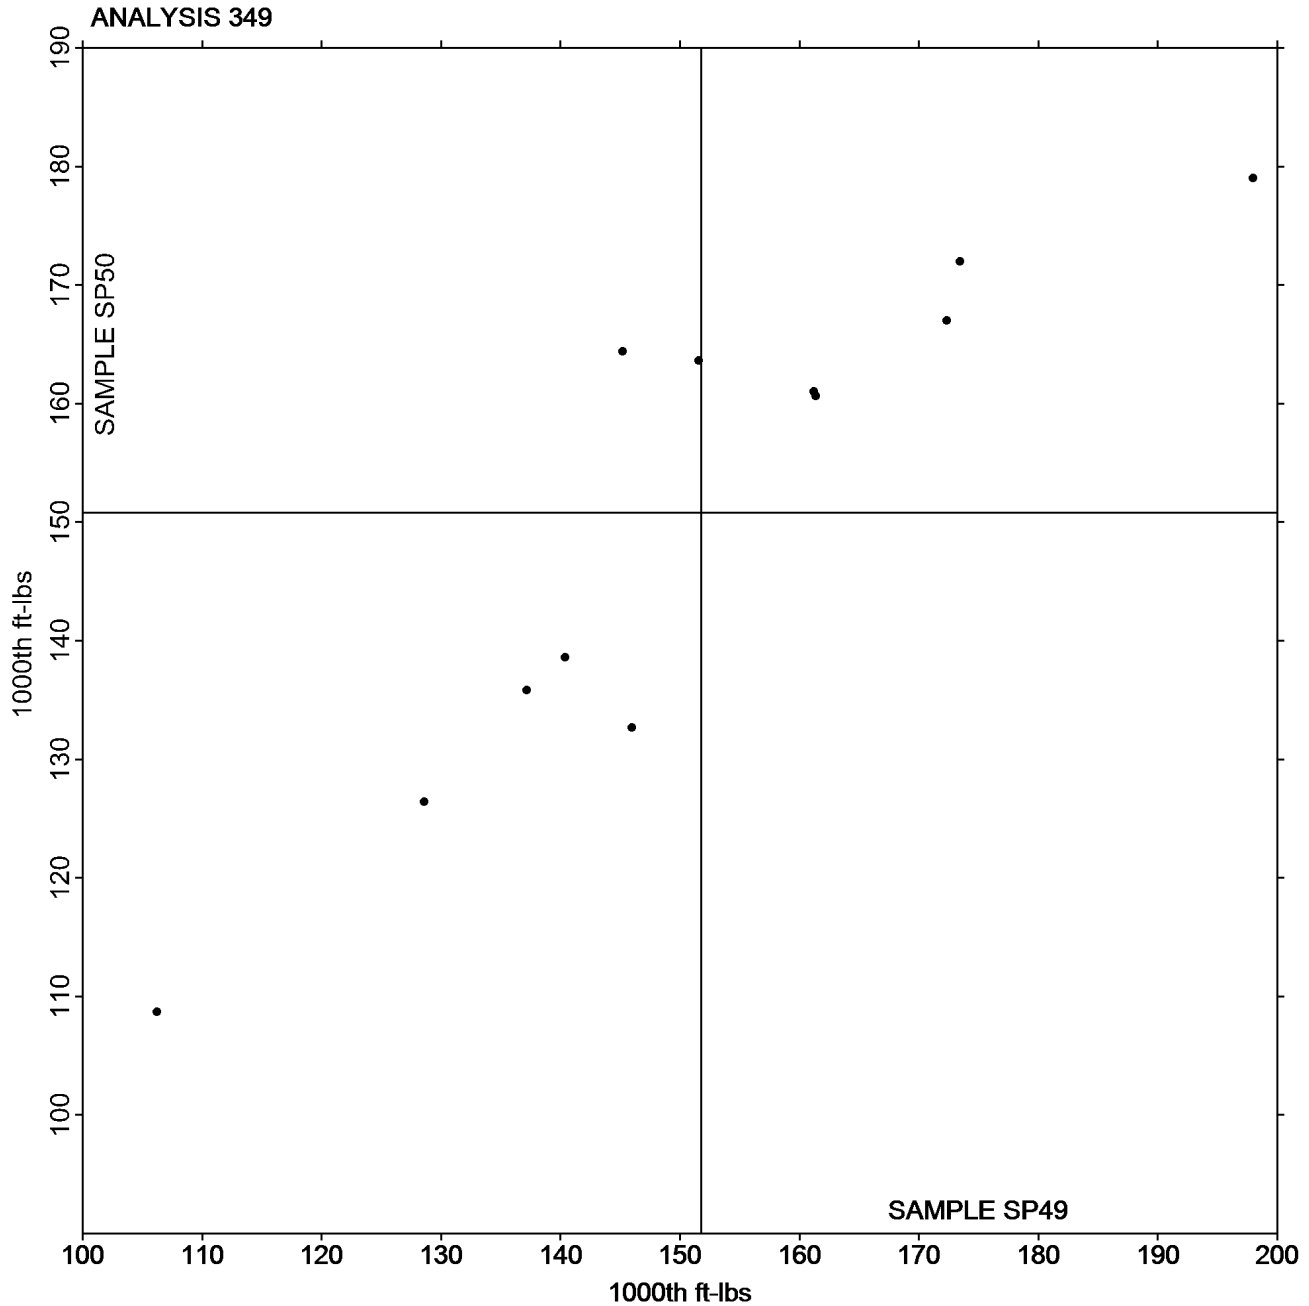

If fewer than 20 laboratories are included in an analysis, a control ellipse will not be drawn on the two-sample plot.